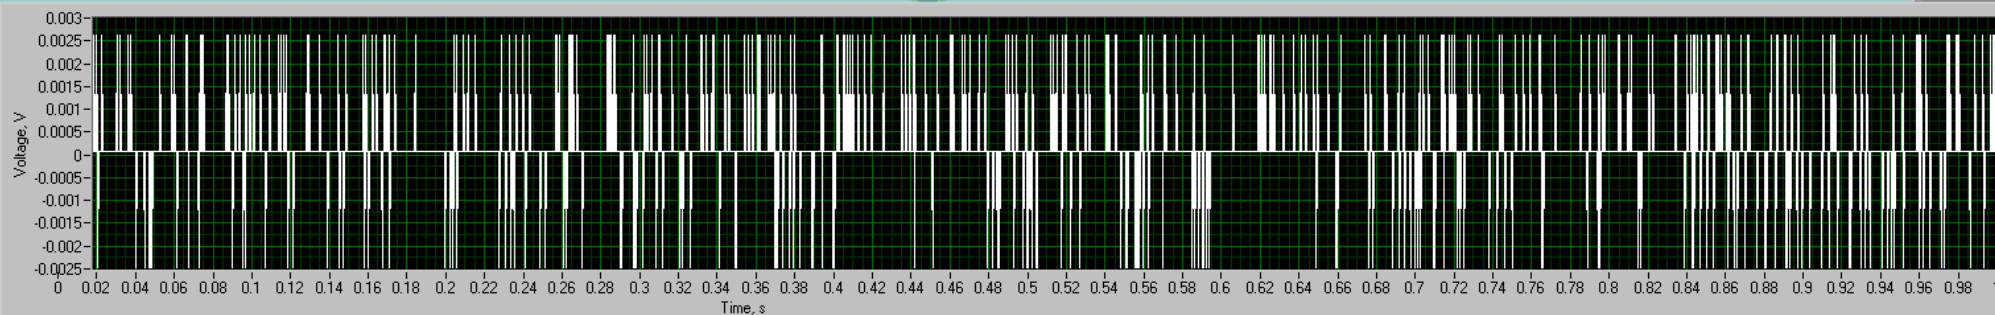


File path C:\KD-test\VC\KD-test\Light-Sheet-Velocimeter\Test 2015-01-15.dat

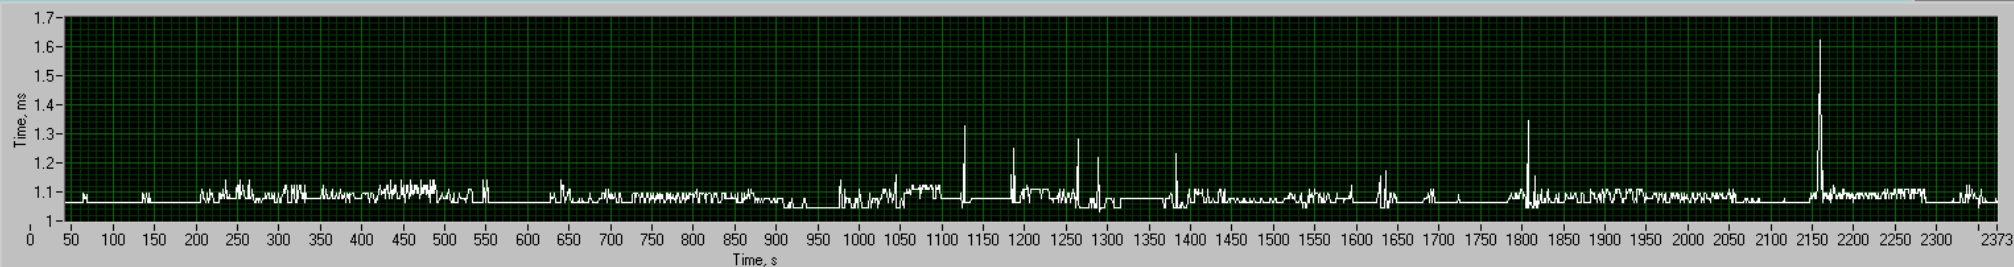

DC Current, A Voltage
0 0Charts reset Counter, s Counter, HH Amps-hours Watt-hours AverCurrent WriteHeader DataAutoSave DataSaving
2562.375 0.711771 0.094047007 0.0000000 0.1321310

Page 1 Page 2 STOP NN samples 4379 Timer, ms 2387348161 TimerPeriod, ms 1062

Input current graph Rate samples/s 10000 NN Of Samples 10000 Input calibration 1.39413 Input zero



Timer Period graph, ms

number of samples
10000pulse duration
0.00Max Voltage, V 0.002632
DC Voltage, V 0.000114
Min Voltage, V -0.002457Max Current
DC Current
Min Current
0 Line

Average and Peak currents Chart

