LRAUV LAB DATA COLLECTION SYSTEM PHASE 2
SEPARATE DAQ HOUSING

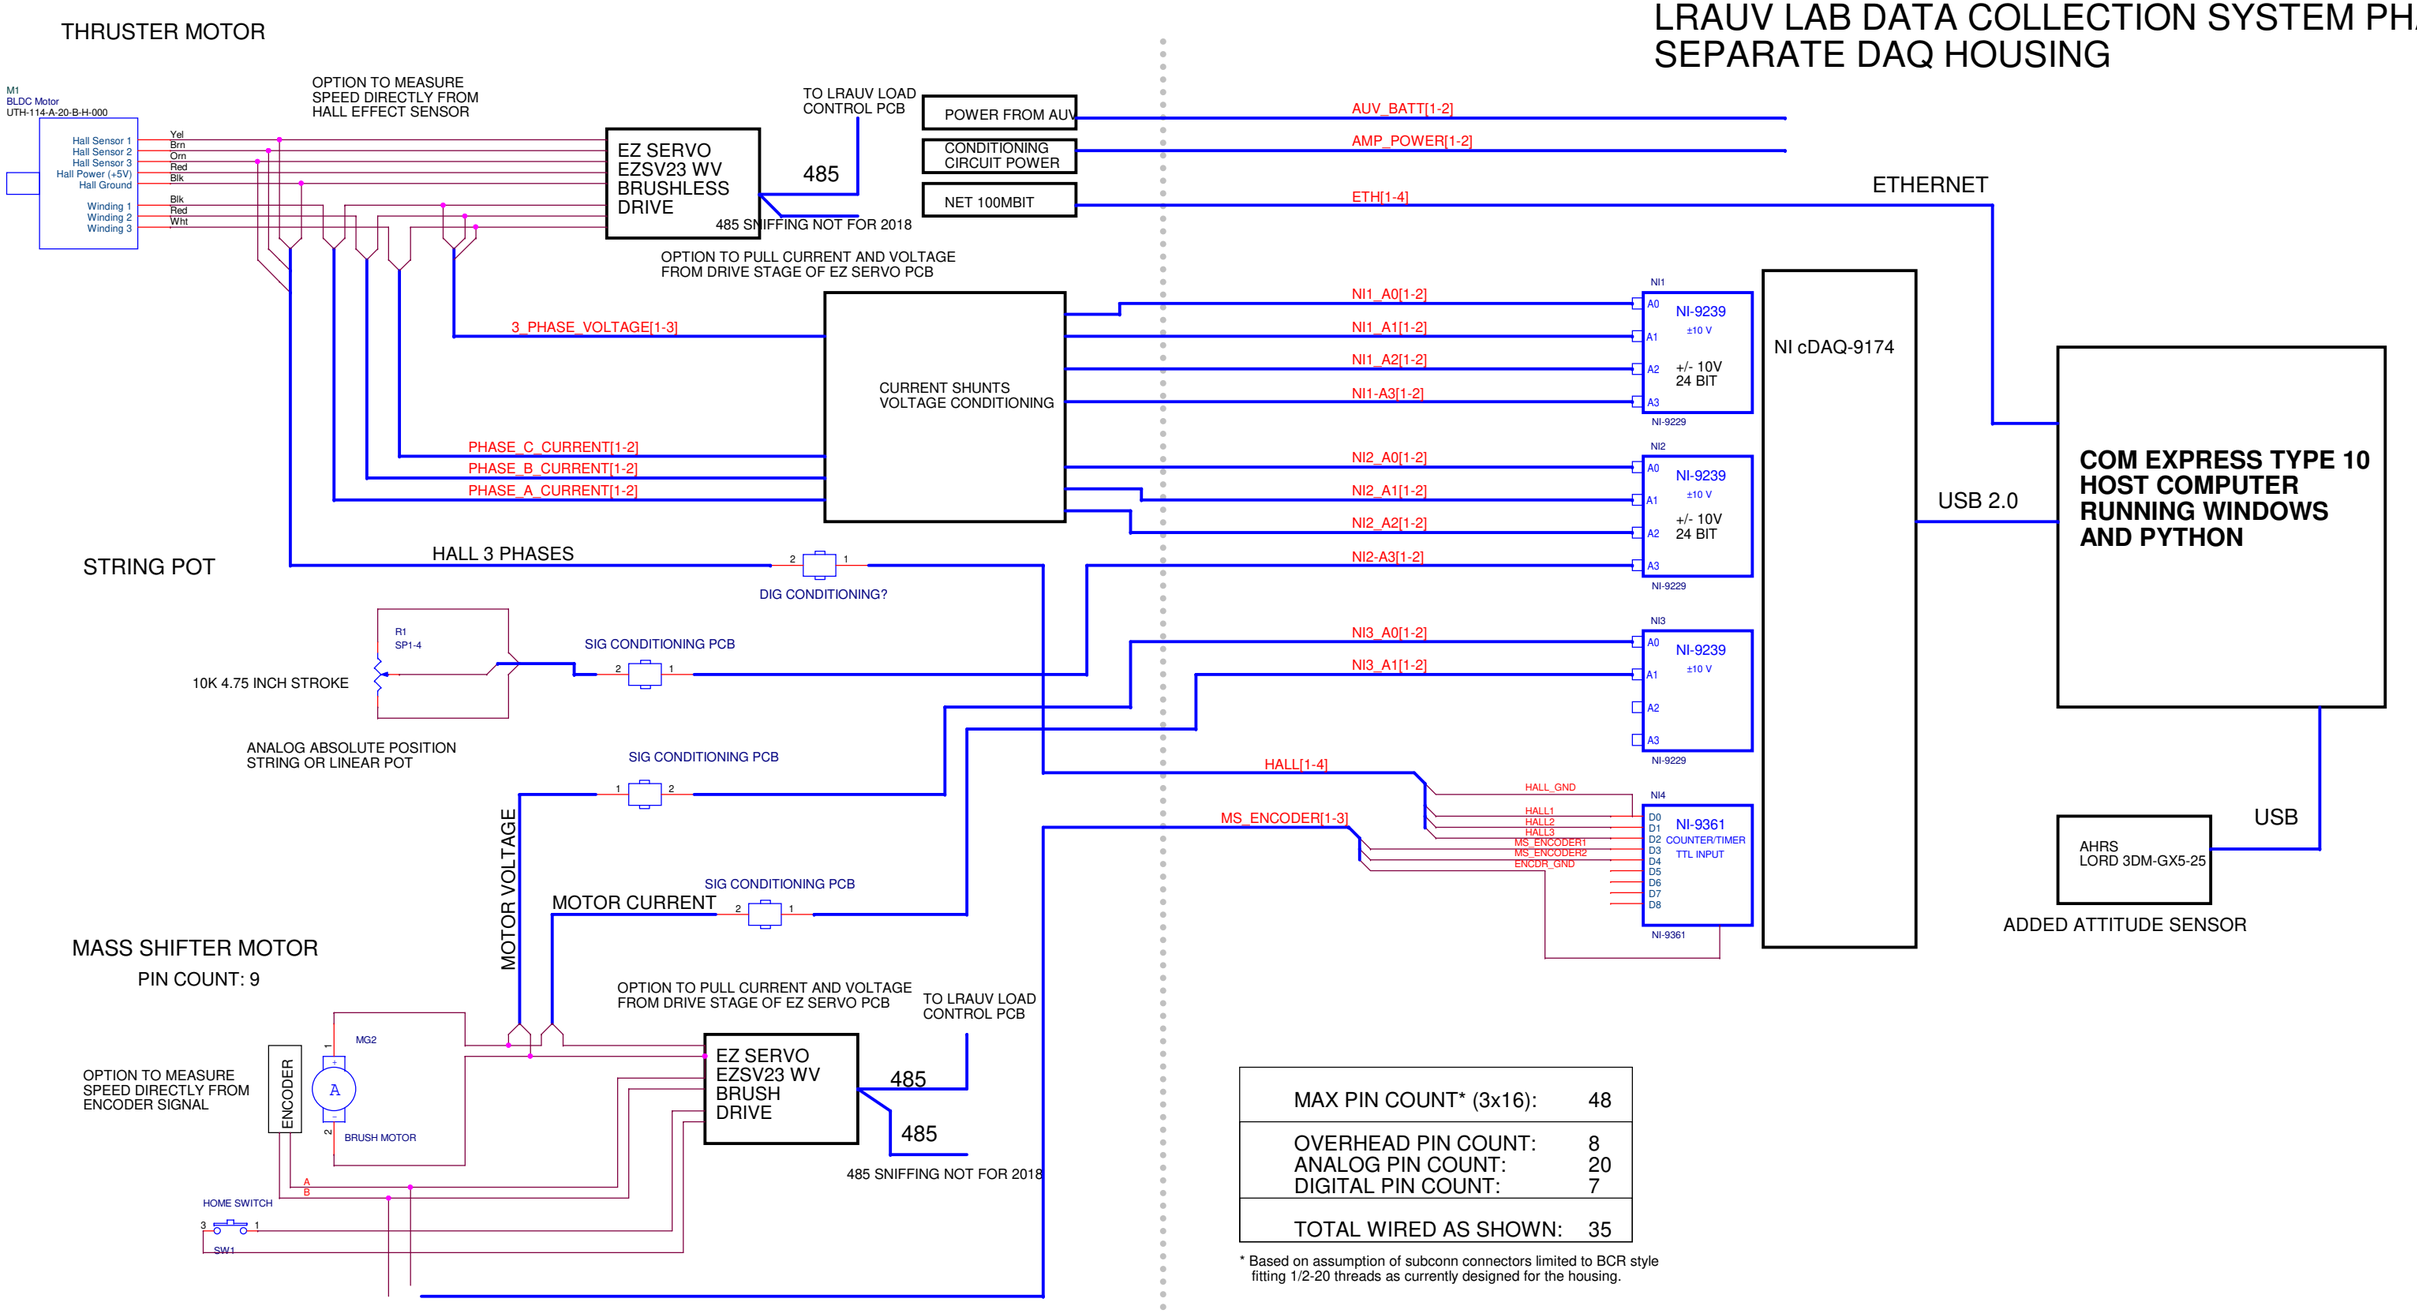

MAX PIN COUNT* (3x16):	48
OVERHEAD PIN COUNT:	8
ANALOG PIN COUNT:	20
DIGITAL PIN COUNT:	7
TOTAL WIRED AS SHOWN:	35

* Based on assumption of subconn connectors limited to BCR style fitting 1/2-20 threads as currently designed for the housing.

MONTEREY BAY AQUARIUM RESEARCH INSTITUTE
7700 SANDHOLDT ROAD
MOSS LANDING, CA 95039
PHONE (831) 775-1700 www.mbari.org

COPYRIGHT © 2018 MBARI
MAY NOT BE COPIED WITHOUT PERMISSION

Title: **LRAUV LAB DATA COLLECTION SYSTEM PHASE 2**

Size	Engineer: Mark Chaffey / Eric Martin, EMAIL: chma@mbari.org (831) 775-1708	Number: 100221234-02	Rev: B
	Date: Thursday, August 23, 2018	Filename: <Filename>	Sheet 1 of 1