

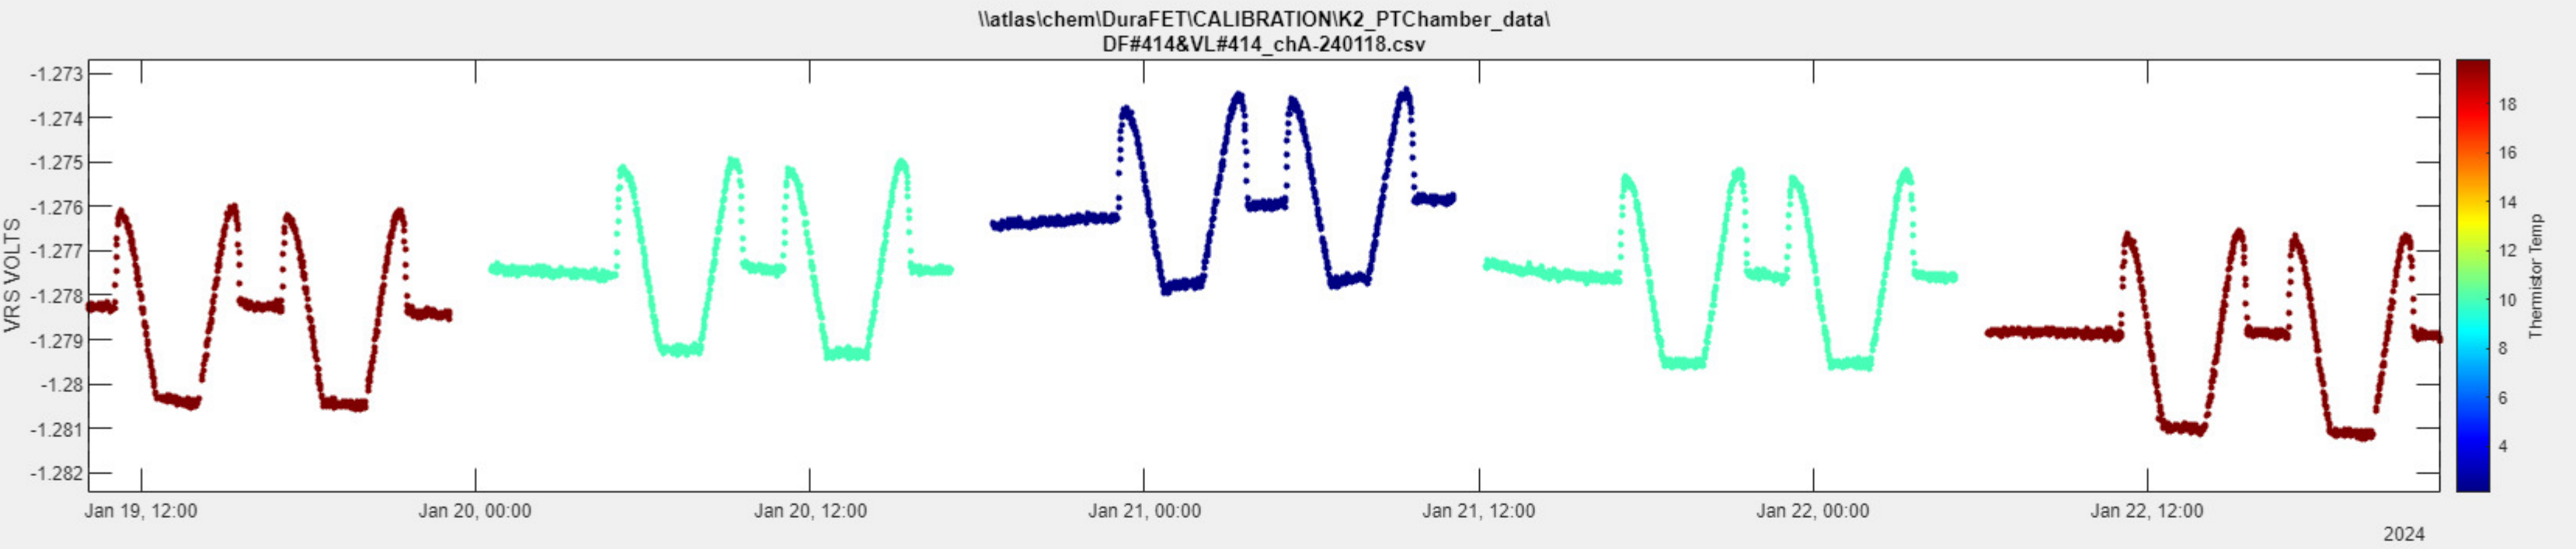


Choose k2 Press chamber file

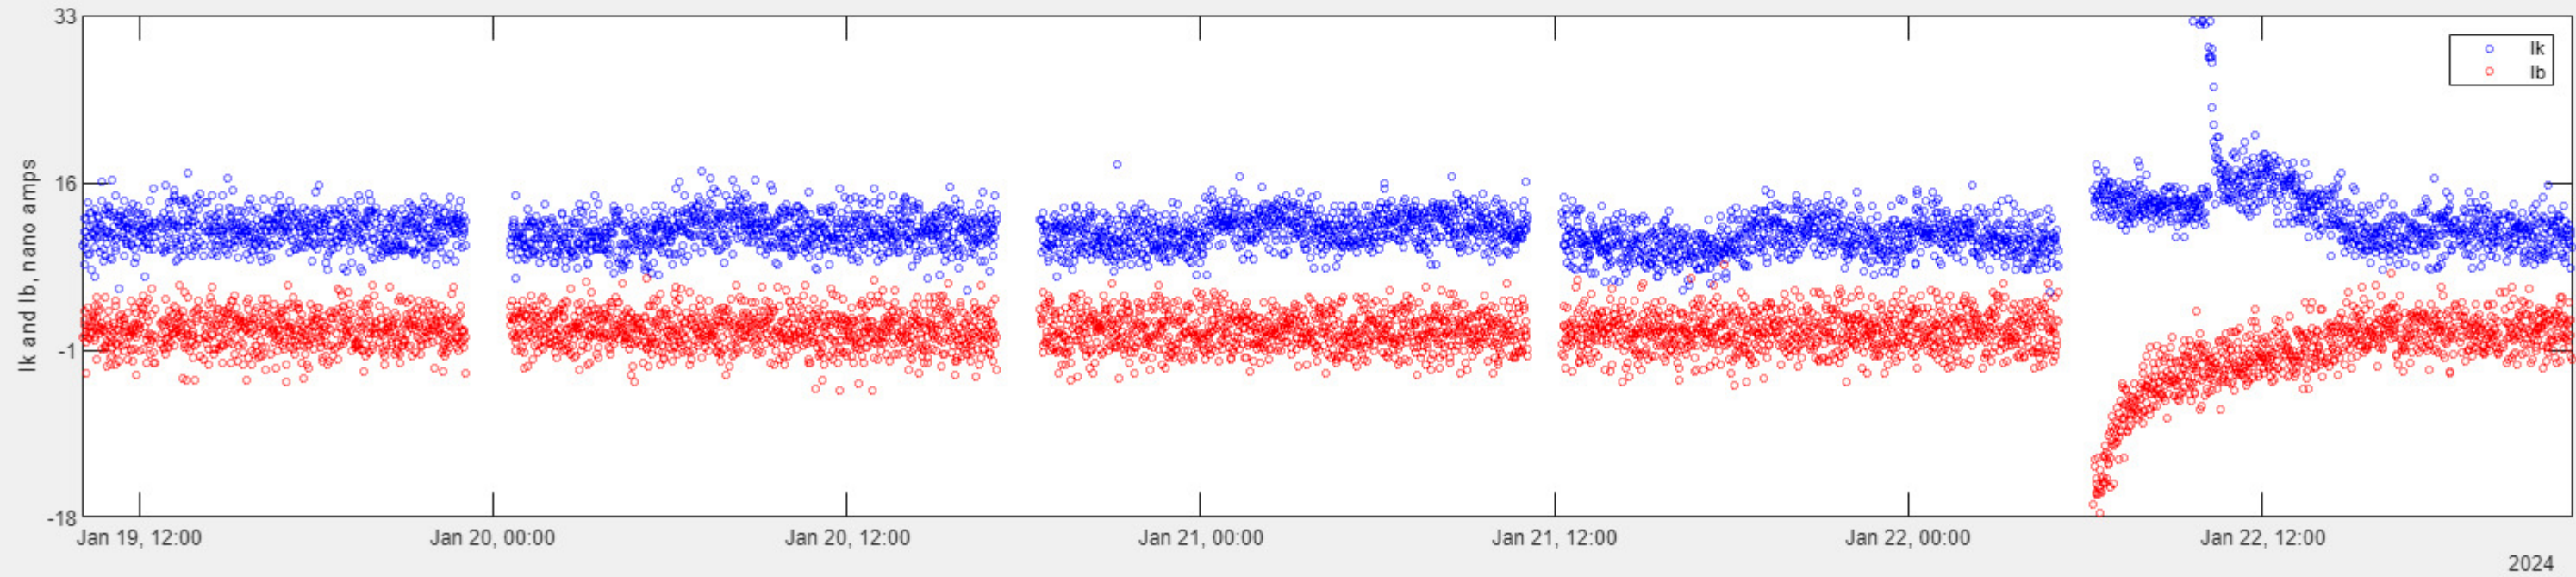

Vk Y axis

- volts
- std volts

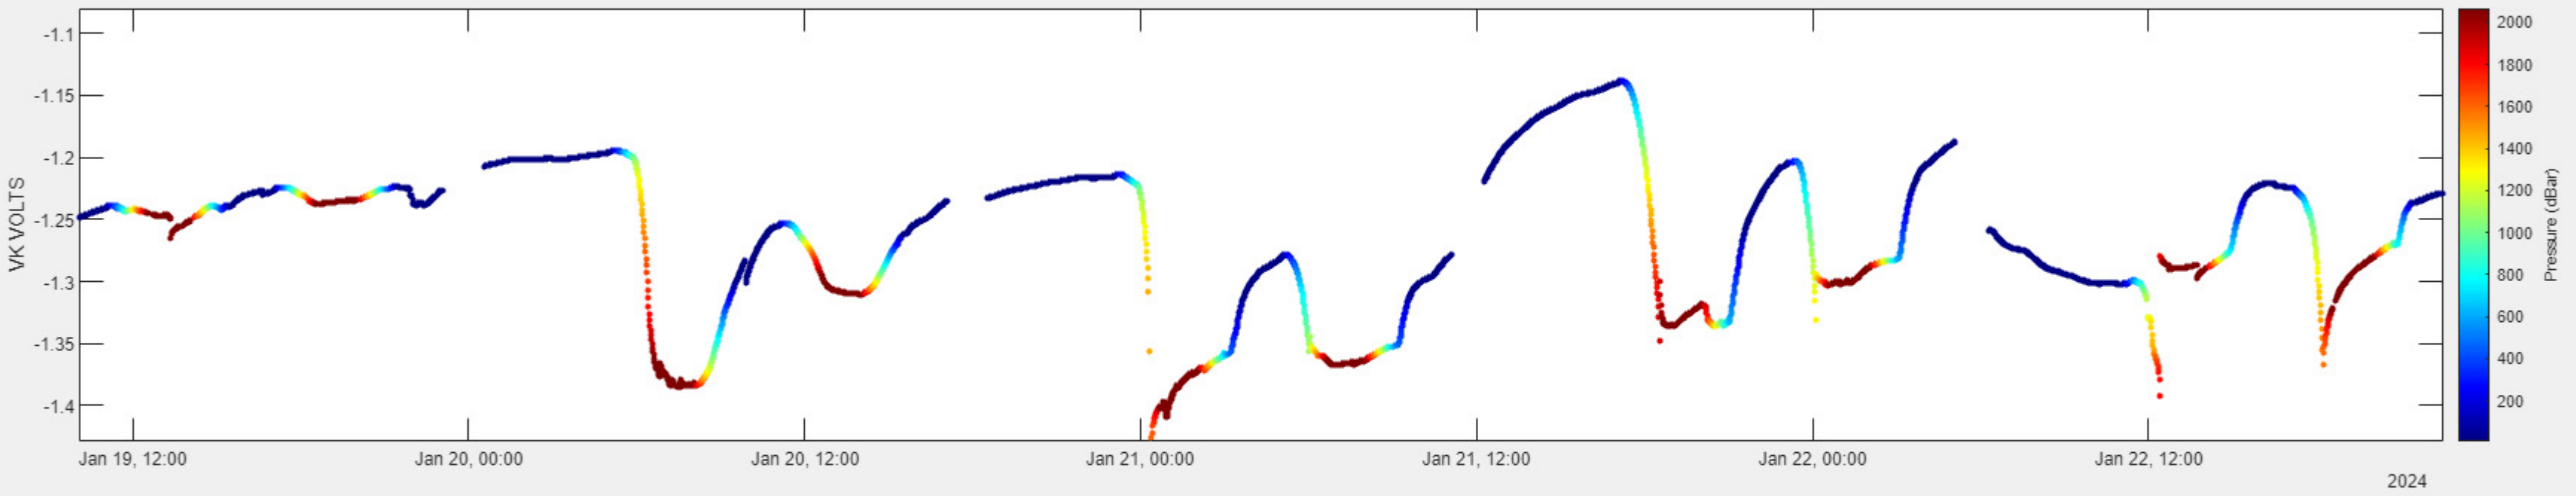


Min

Max

Jan 19 10:07

Jan 22 22:29

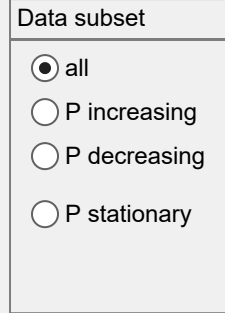

Sensor SN not in pH log file!!!!		
Process Date:	01/23/2024 13:15	
Durafet SN:	414	
pH stem mfg:	MBARI	DF
MSC #:	XXXX	
PT Source directory :	\\atlas\chem\DuraFET\CALIBRATION\K2_PTCha...	
PT Source file :	DF#414&VL#414_chA-240118.csv	
PT test channel :	A	
HCl concentration:	0.01000	Molar
k2 Calibration window:	01/19/2024 10:07	01/22/2024 22:29
Data subset:	ALL	
Vrs drift rate:	-0.19494	mV/day
Vk drift rate:	-9.48505	mV/day
Avg std Vk	89.96716	uVolts
Average k2:	-9.6342e-04	V/degC
Std dev k2:	5.0339e-06	V/degC
k2 f(P) c0	-9.6342e-04	
k2 f(P) c1	0.0000e+00	
k0 HCL:	-1.4971	Volts
Avg Ik:	11.39	nano amps
Std dev Ik:	2.33	nano amps
Avg Ib:	0.47	nano amps
Std dev Ib:	2.59	nano amps
f(P) NSSR:	4.9563e-08	
f(P) R*R:	0.9653	
f(P) c0	-1.4970e+00	
f(P) c1	3.1587e-05	
f(P) c2	-1.4149e-07	
f(P) c3	3.4662e-10	
f(P) c4	-4.9517e-13	
f(P) c5	4.1960e-16	
f(P) c6	-2.0752e-19	
f(P) c7	5.5291e-23	
f(P) c8	-6.1286e-27	

Building Report...

poly order



Color Axis

Temperature

Time

Vk

Direction

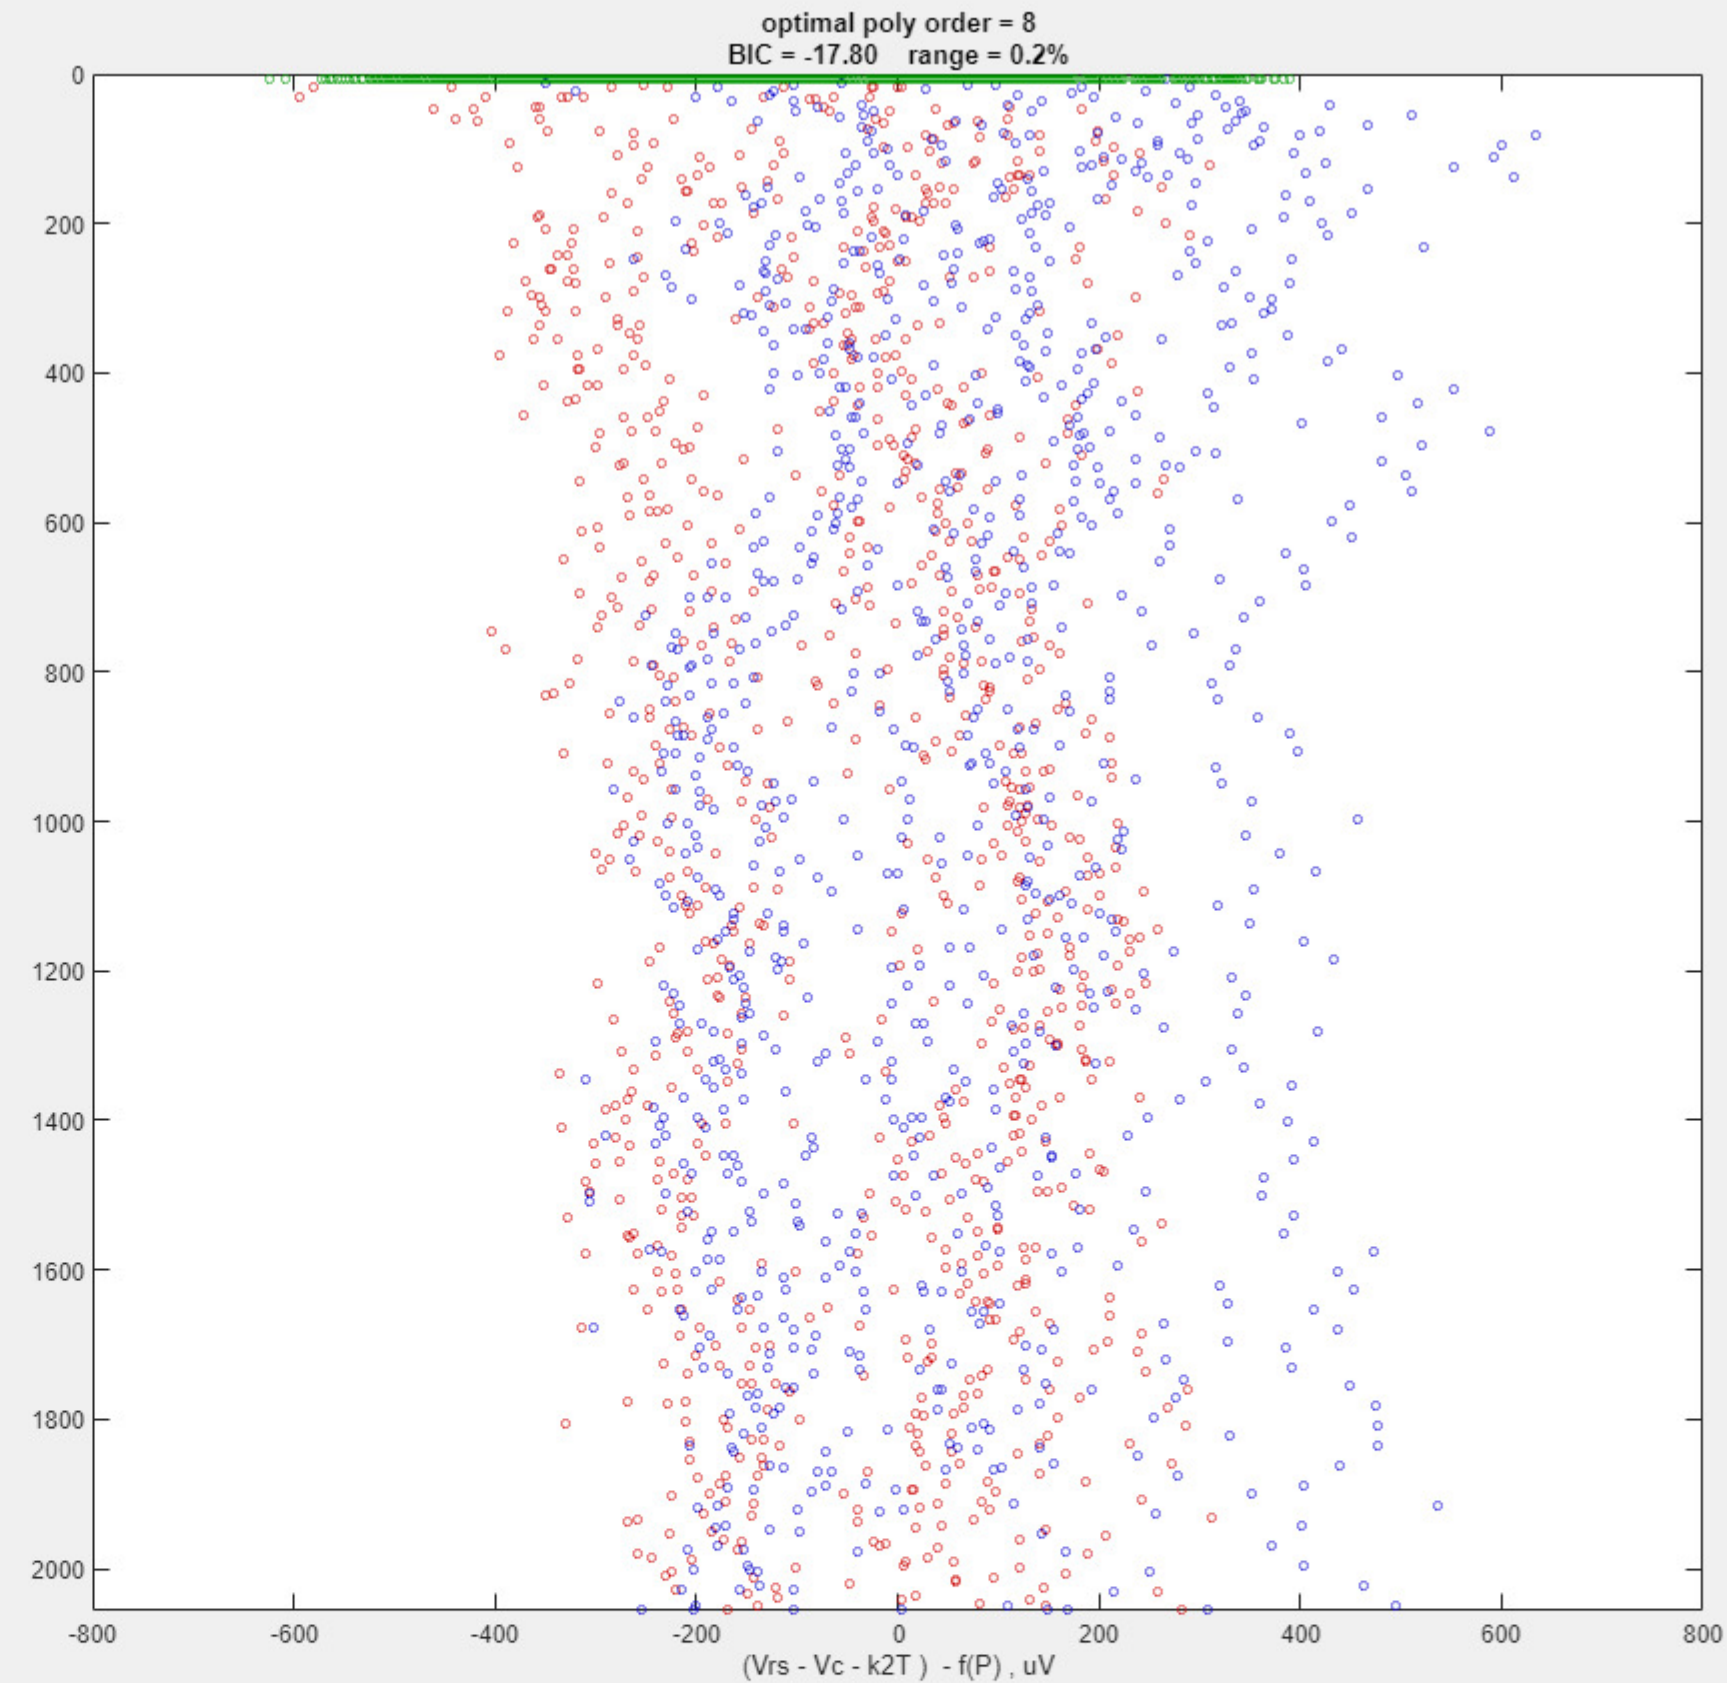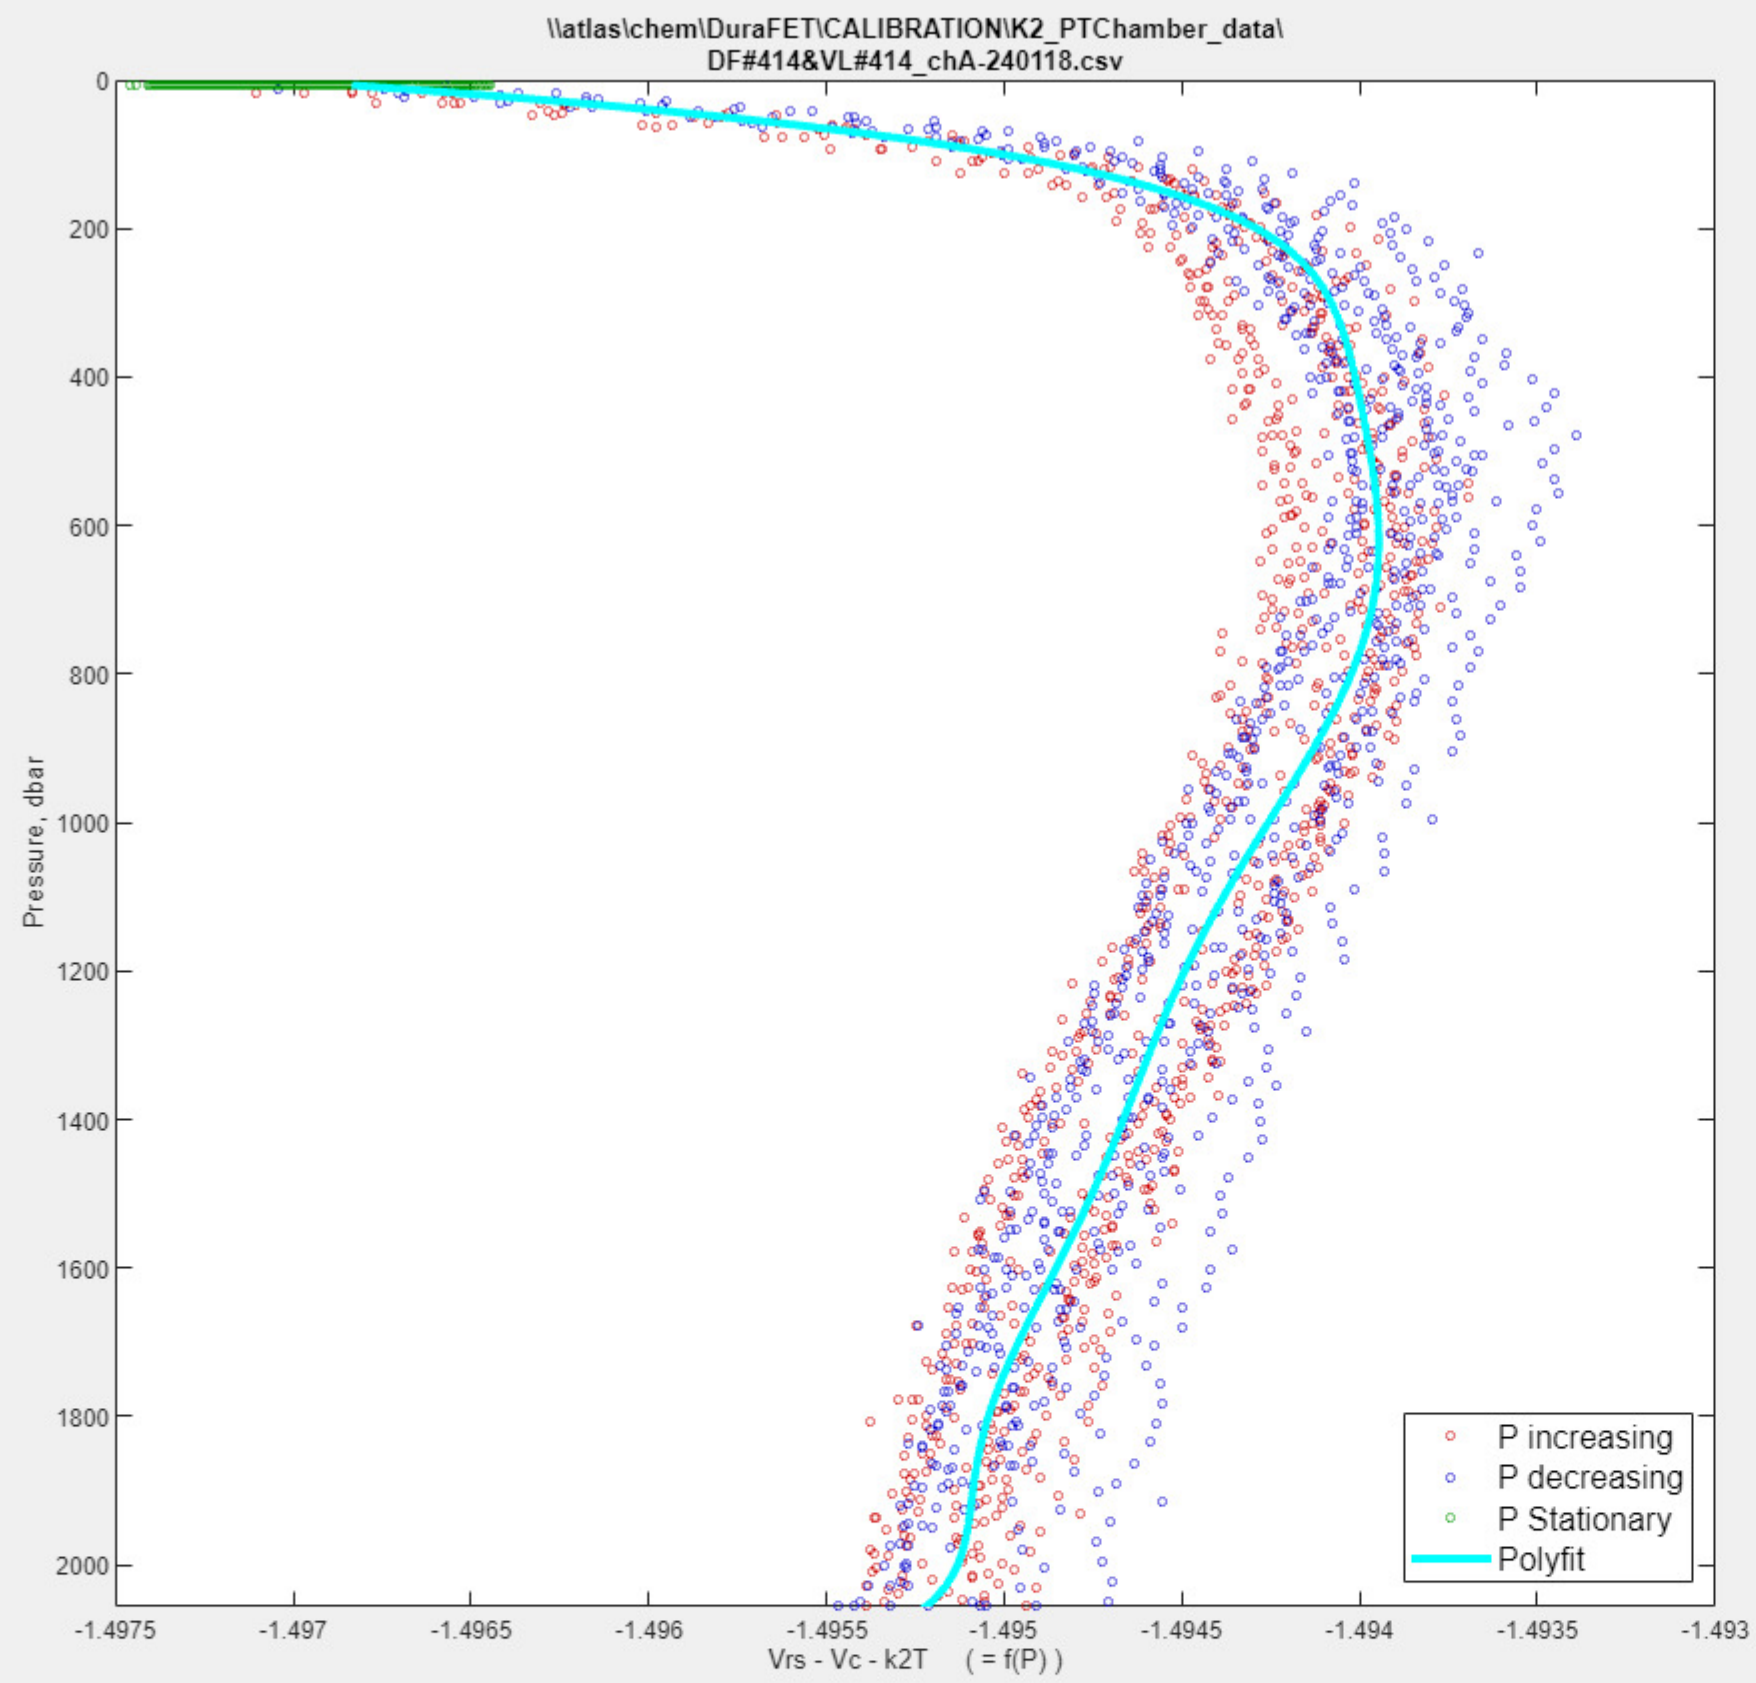

Y axis surface zoom

