






pH
Vernier
Tris-Compatible
pH Sensor
PN# FPH-BTA

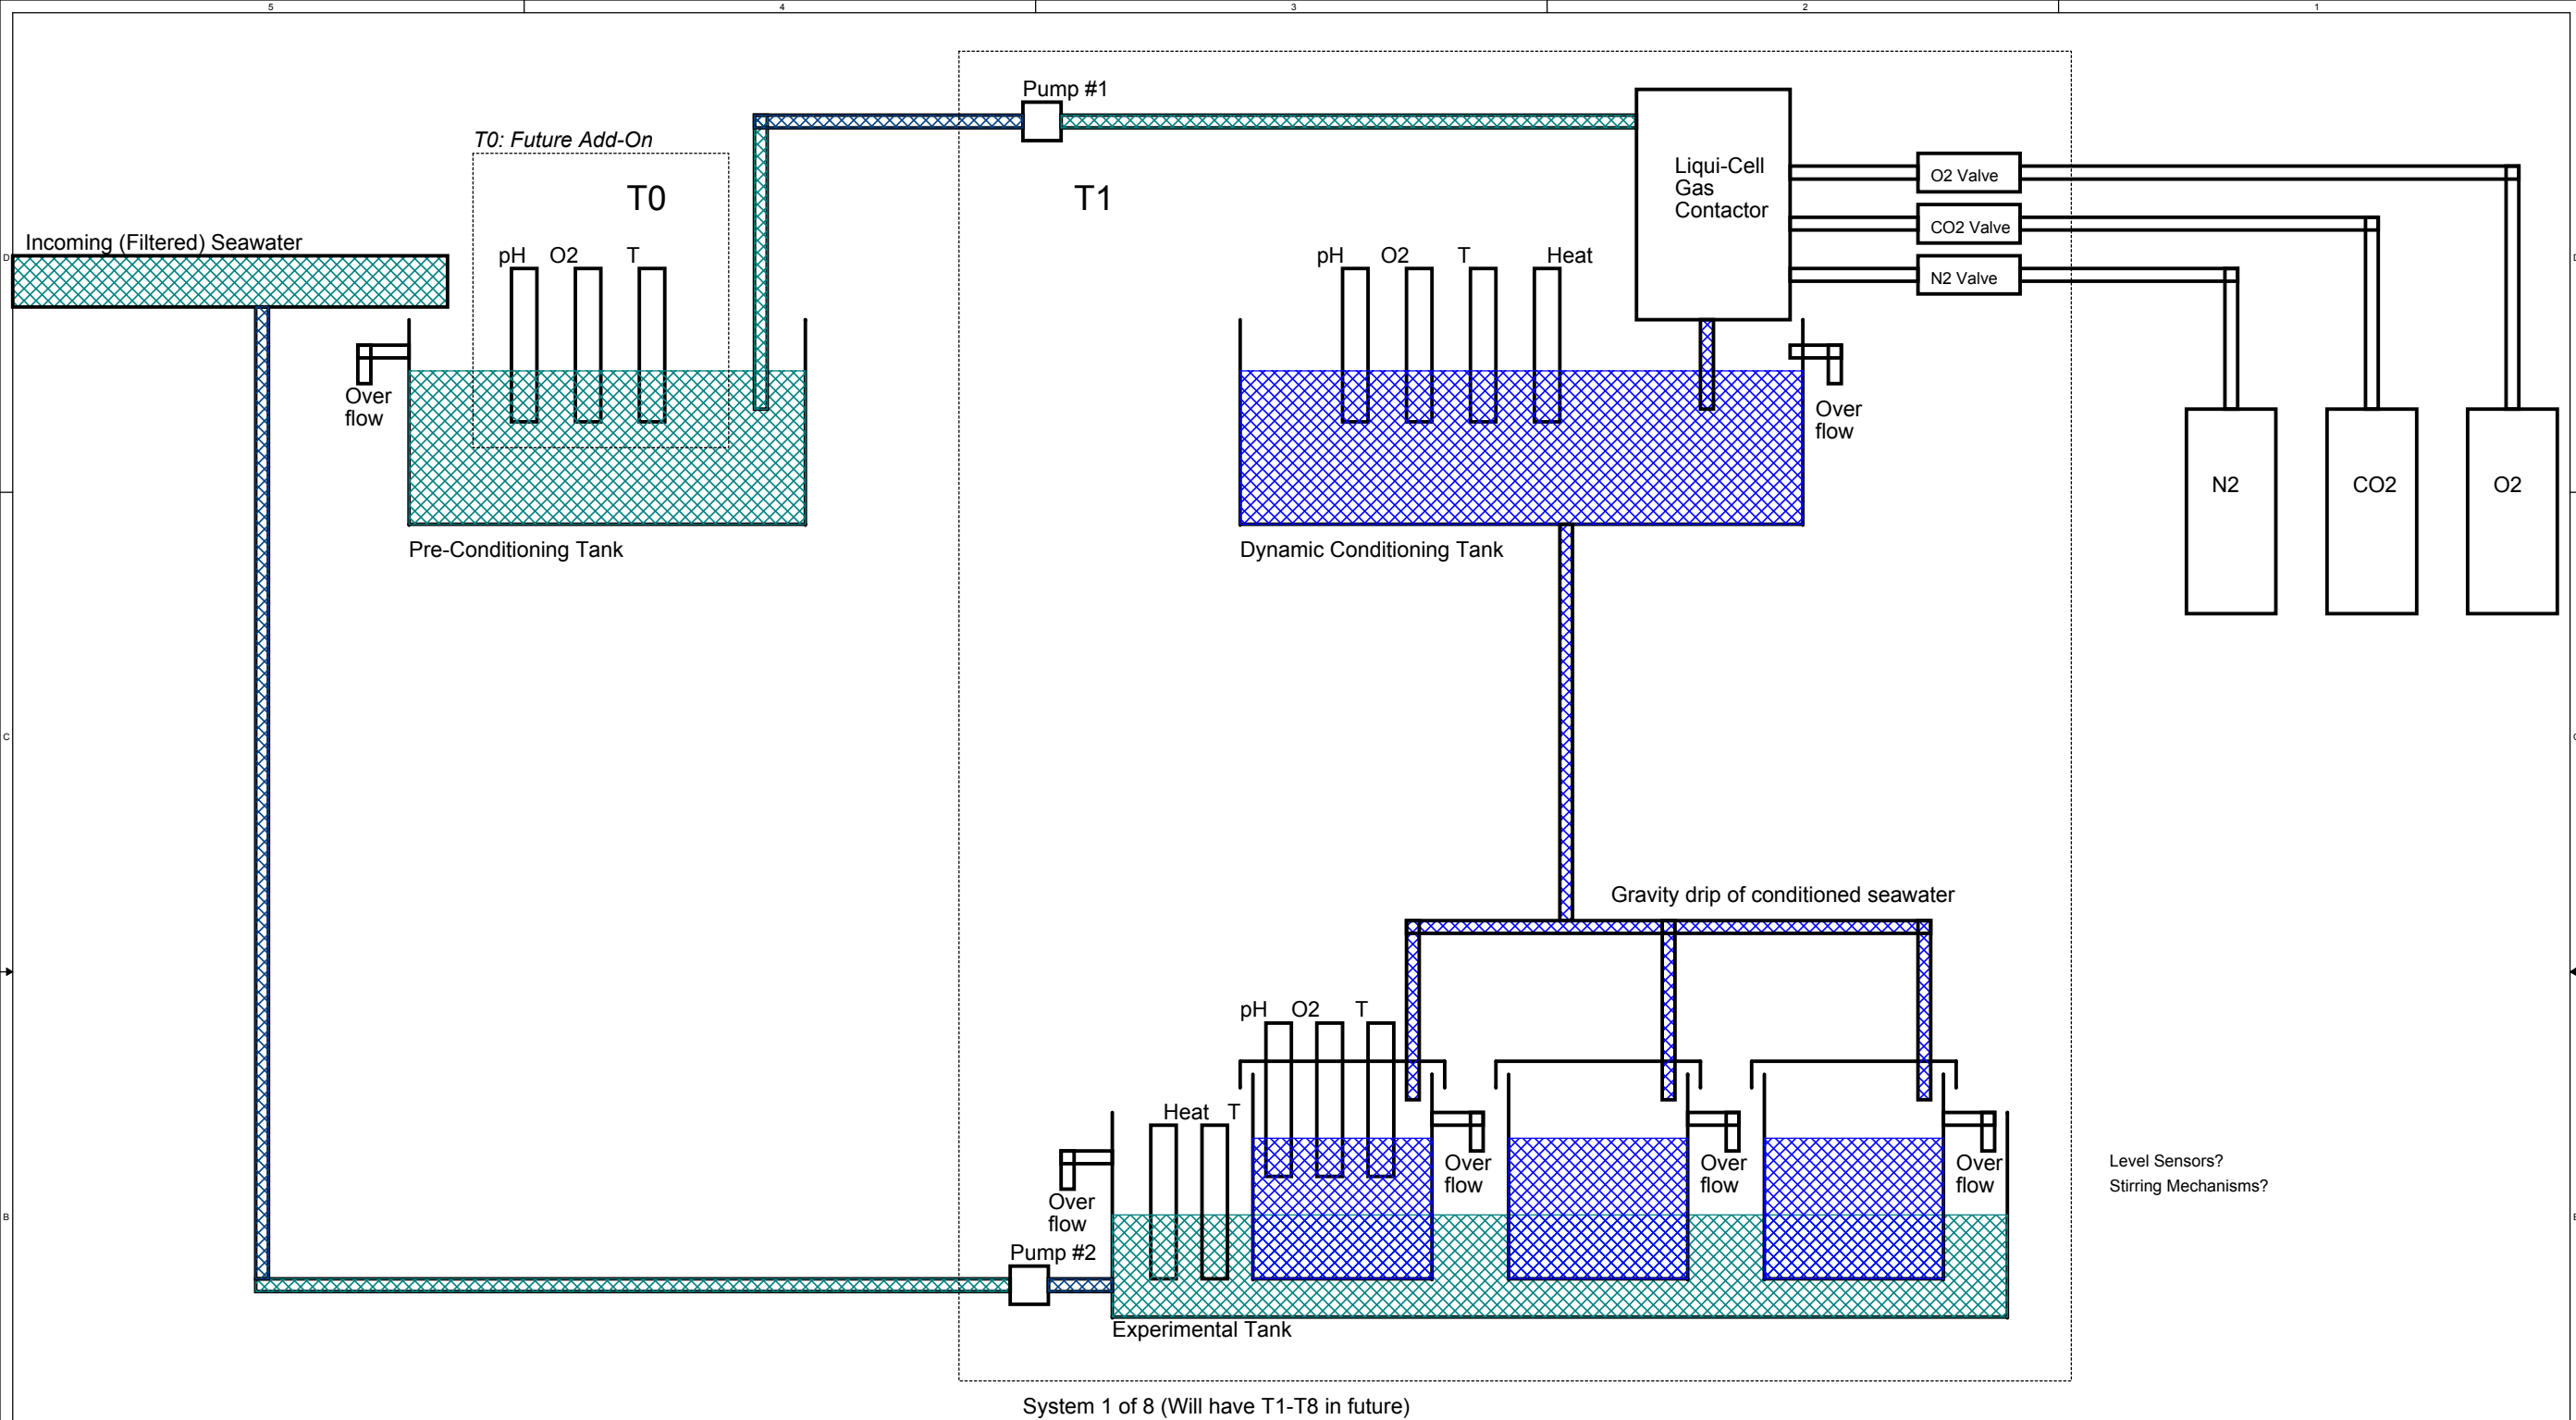

O2
Vernier
Optical
DO Probe
PN# ODO-BTA



T
Omega
PT100
RTD Thermal Probe
PN# PR-22-3-100-A-1/4-0900-M12



Heat
Tempco
Cartridge, 120VAC, 750W
Immersion Heater
PN# HDL00041



xx
Valve
Clippard
EVP Proportional
Solenoid Valve
PN# EC-P-10-2550



Pump #y

MONTEREY BAY AQUARIUM RESEARCH INSTITUTE
7700 SANDHOLDT ROAD
MOSS LANDING, CA 95039
(831) 775-1700 www.mbari.org
Copyright MBARI 2000



Title	Upwelling Aquaria Exp Block Diagram	Number	
Size	Engineer Chad Kacy	Layout <Layout Eng.>	Filename <Filename>
C	Date: Wednesday, February 03, 2016	Sheet 1 of 1	Rev B