





**LMRK60LX-490-15**


**Test Data**

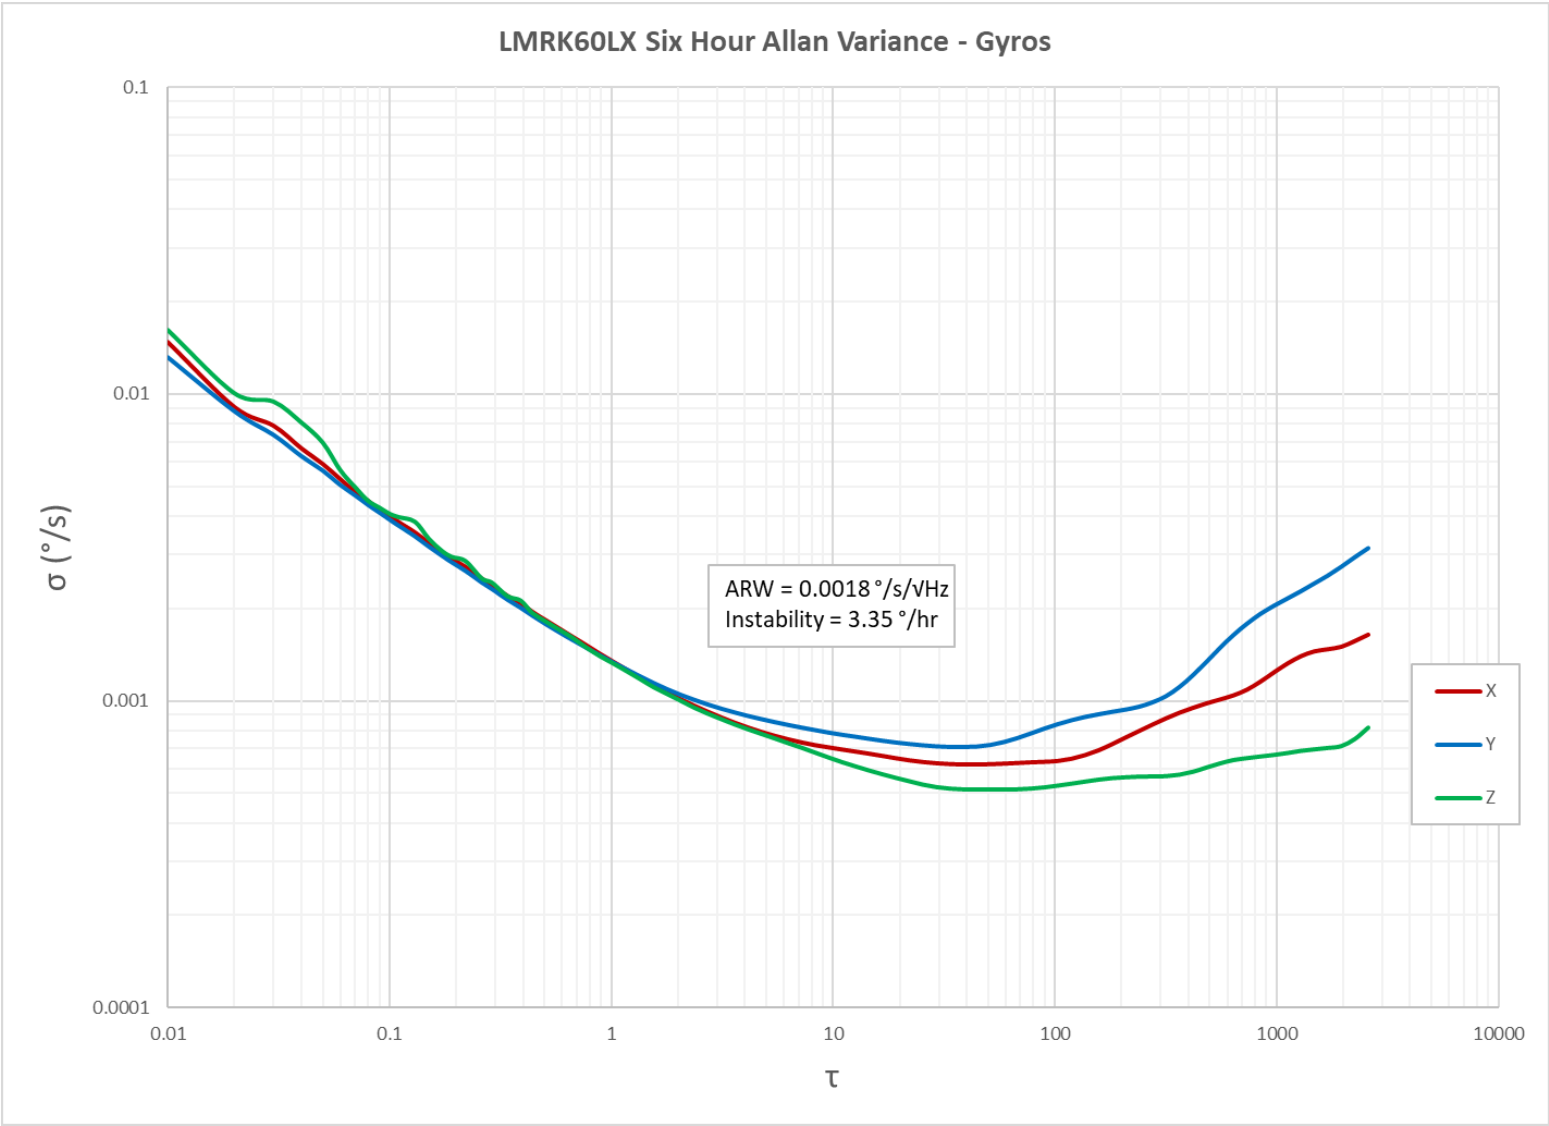


Gyroscope Allan-Variance (limited to 45 minutes)

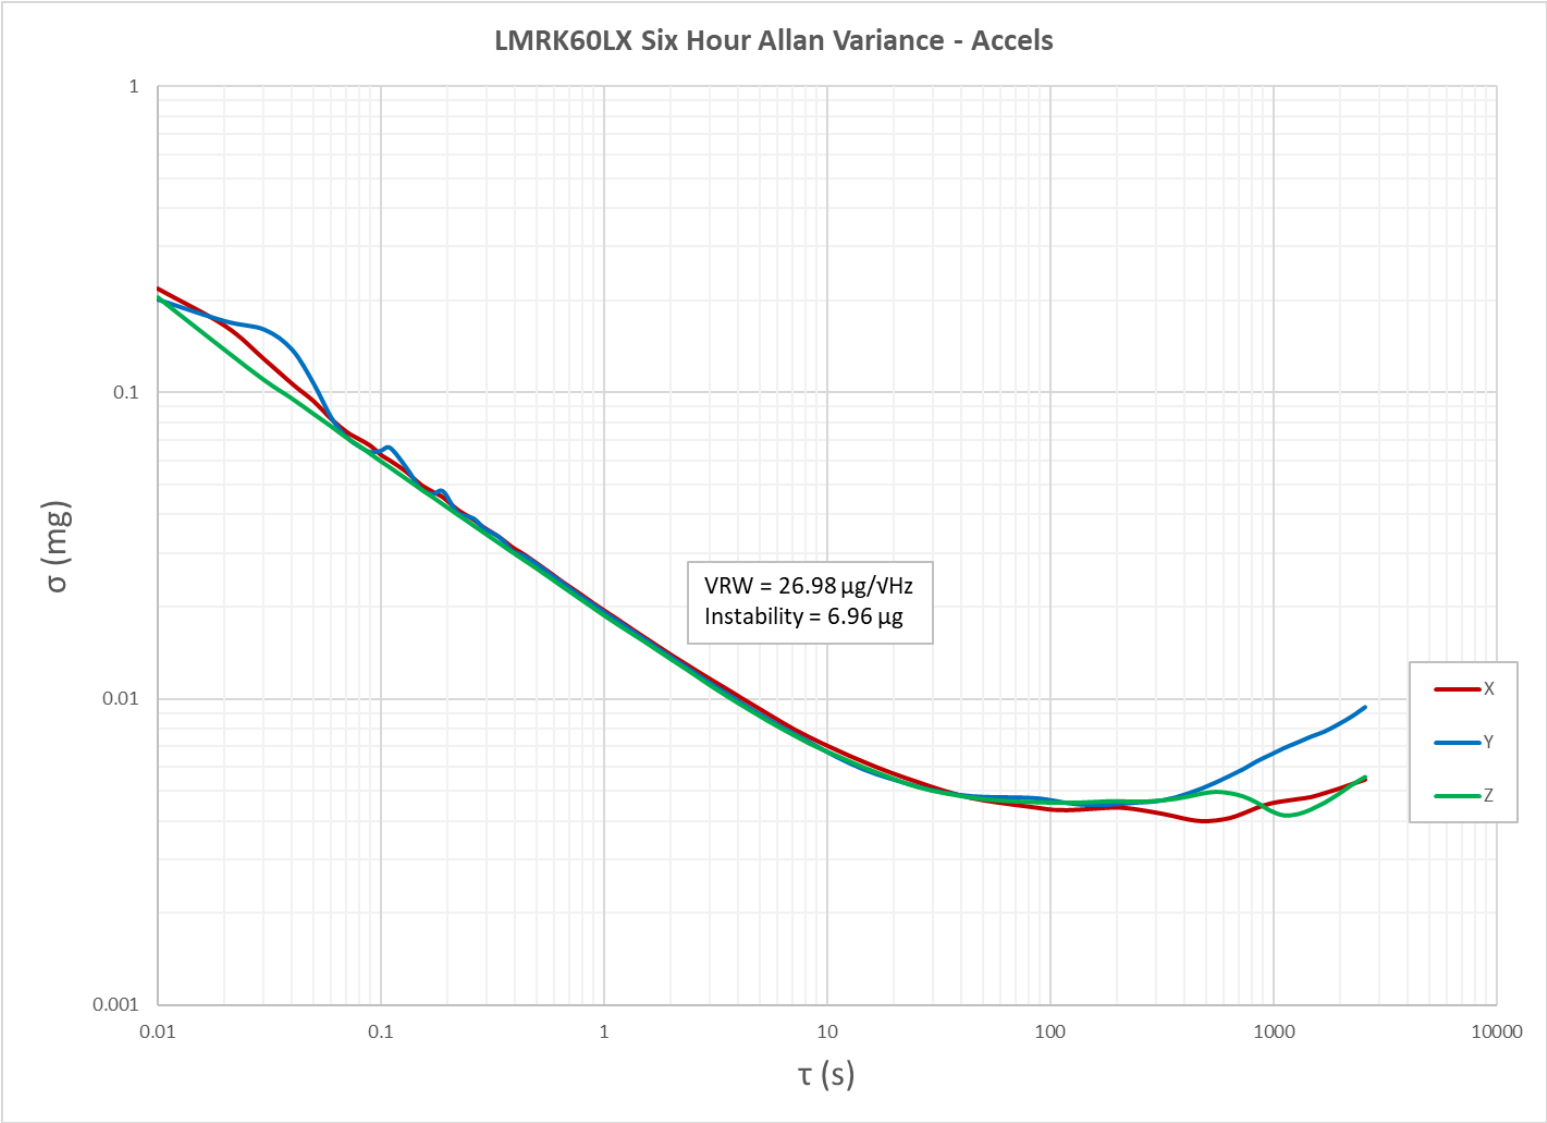


Accelerometer Allan-Variance (limited to 45 minutes)

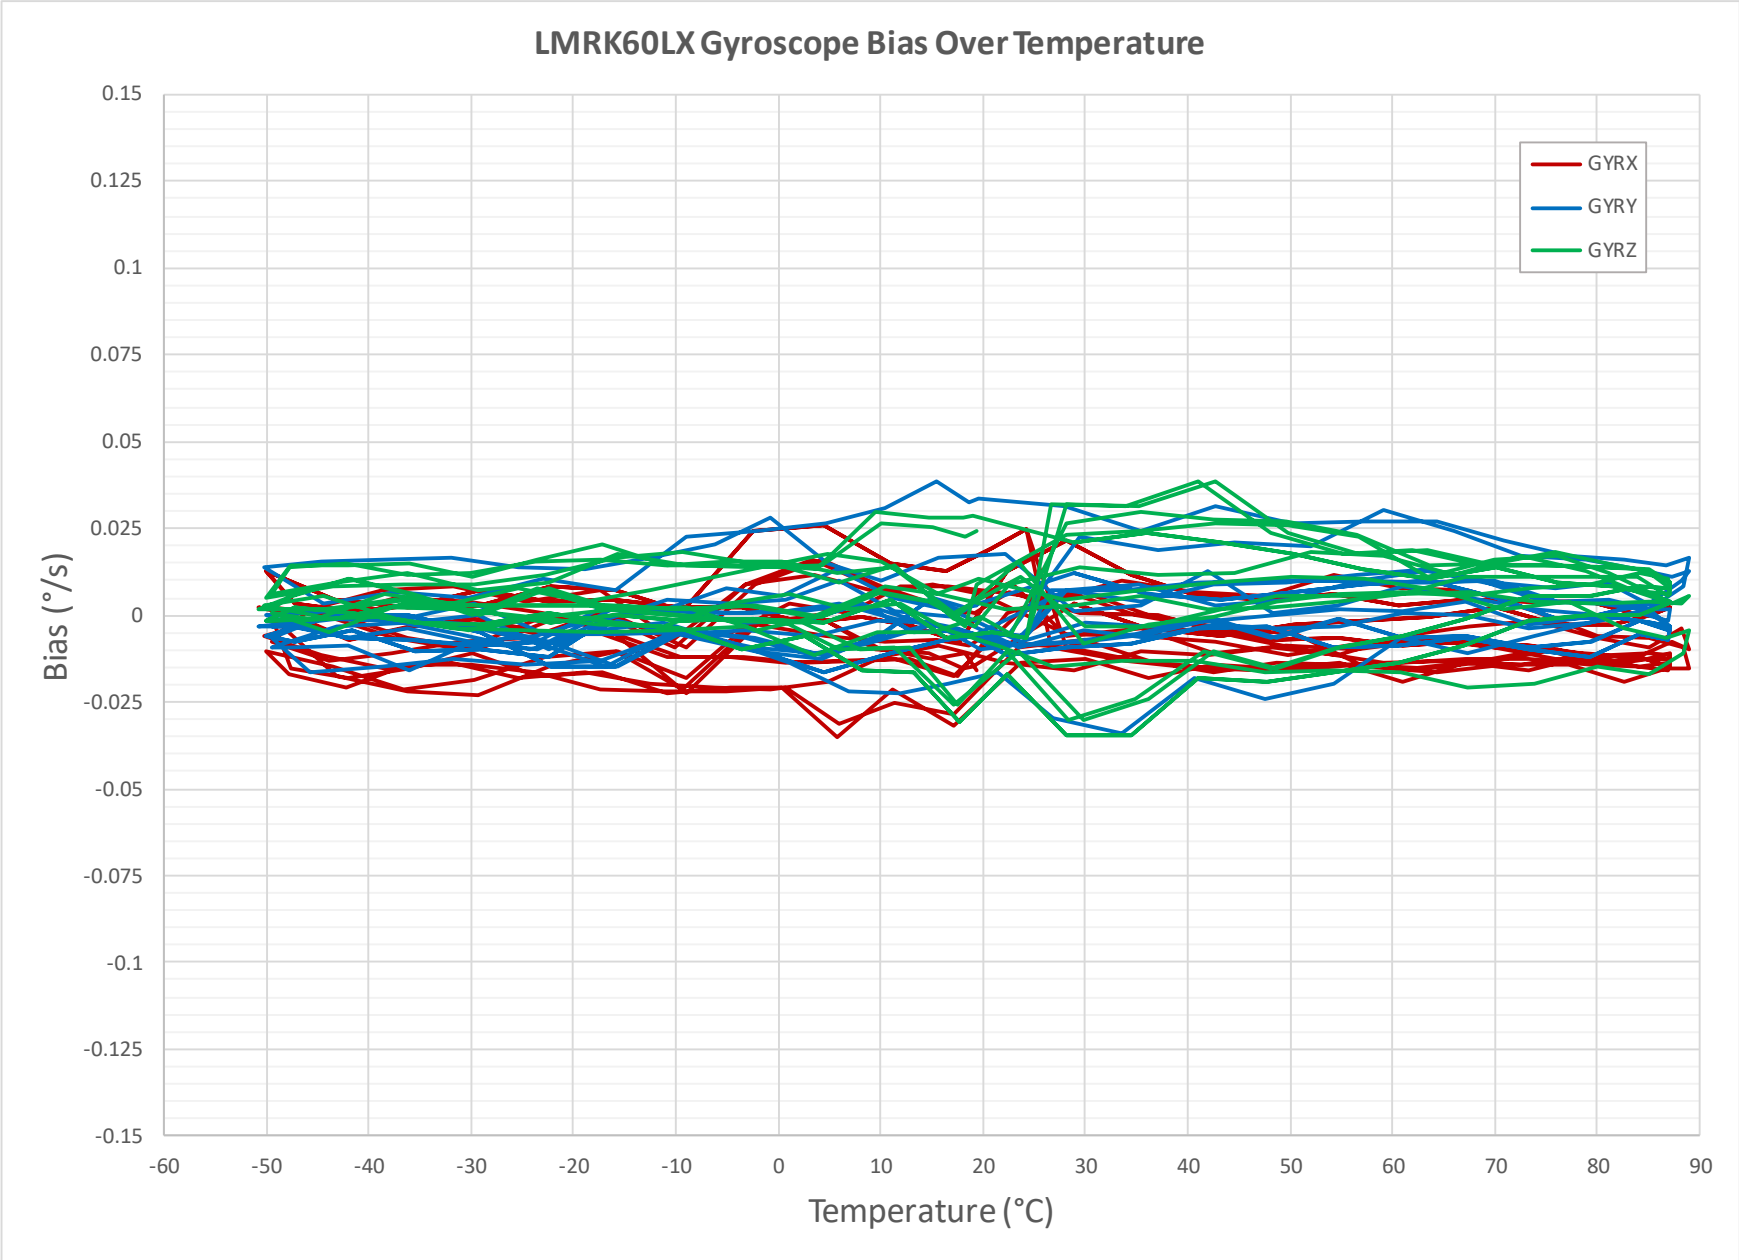


Raw gyroscope output bias over calibrated temperature range

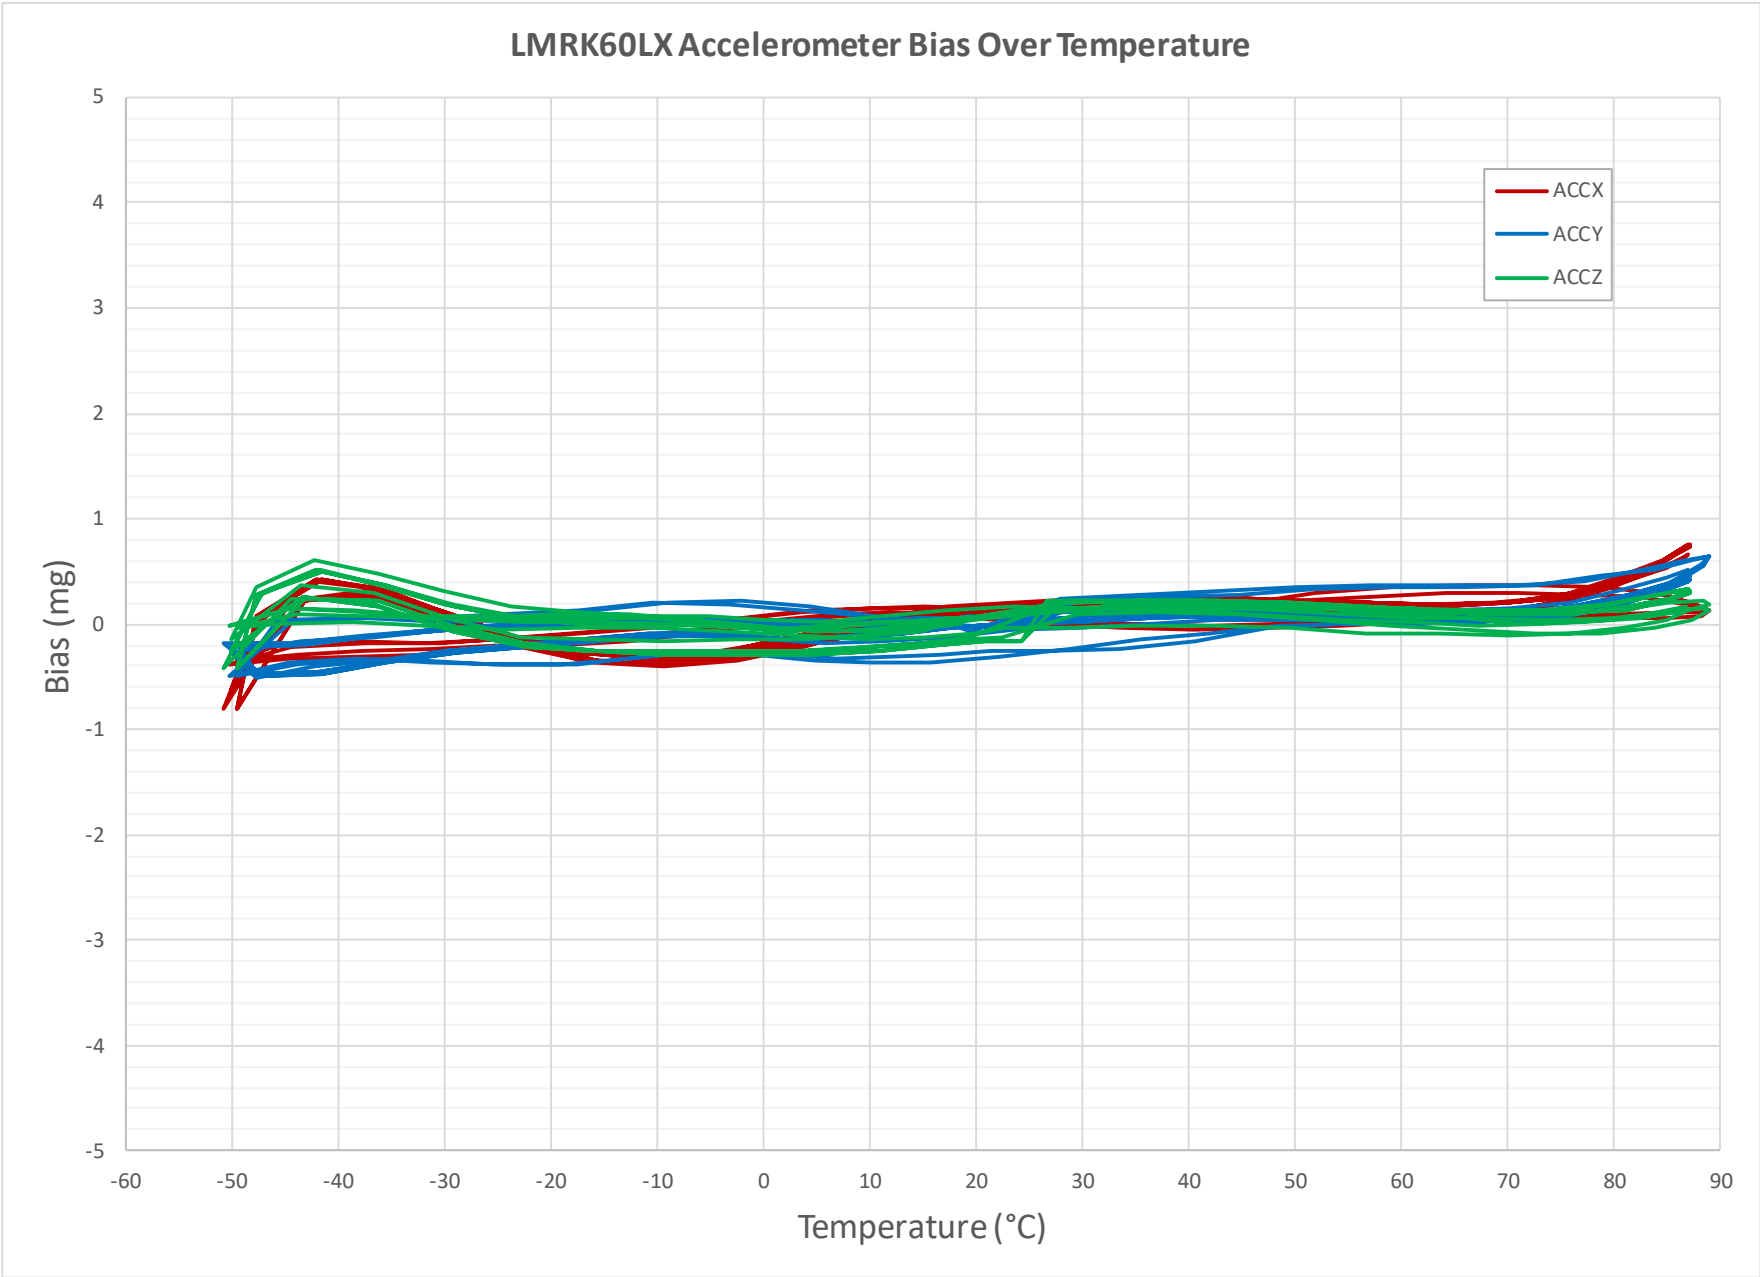

Normalized accelerometer bias over calibrated temperature range

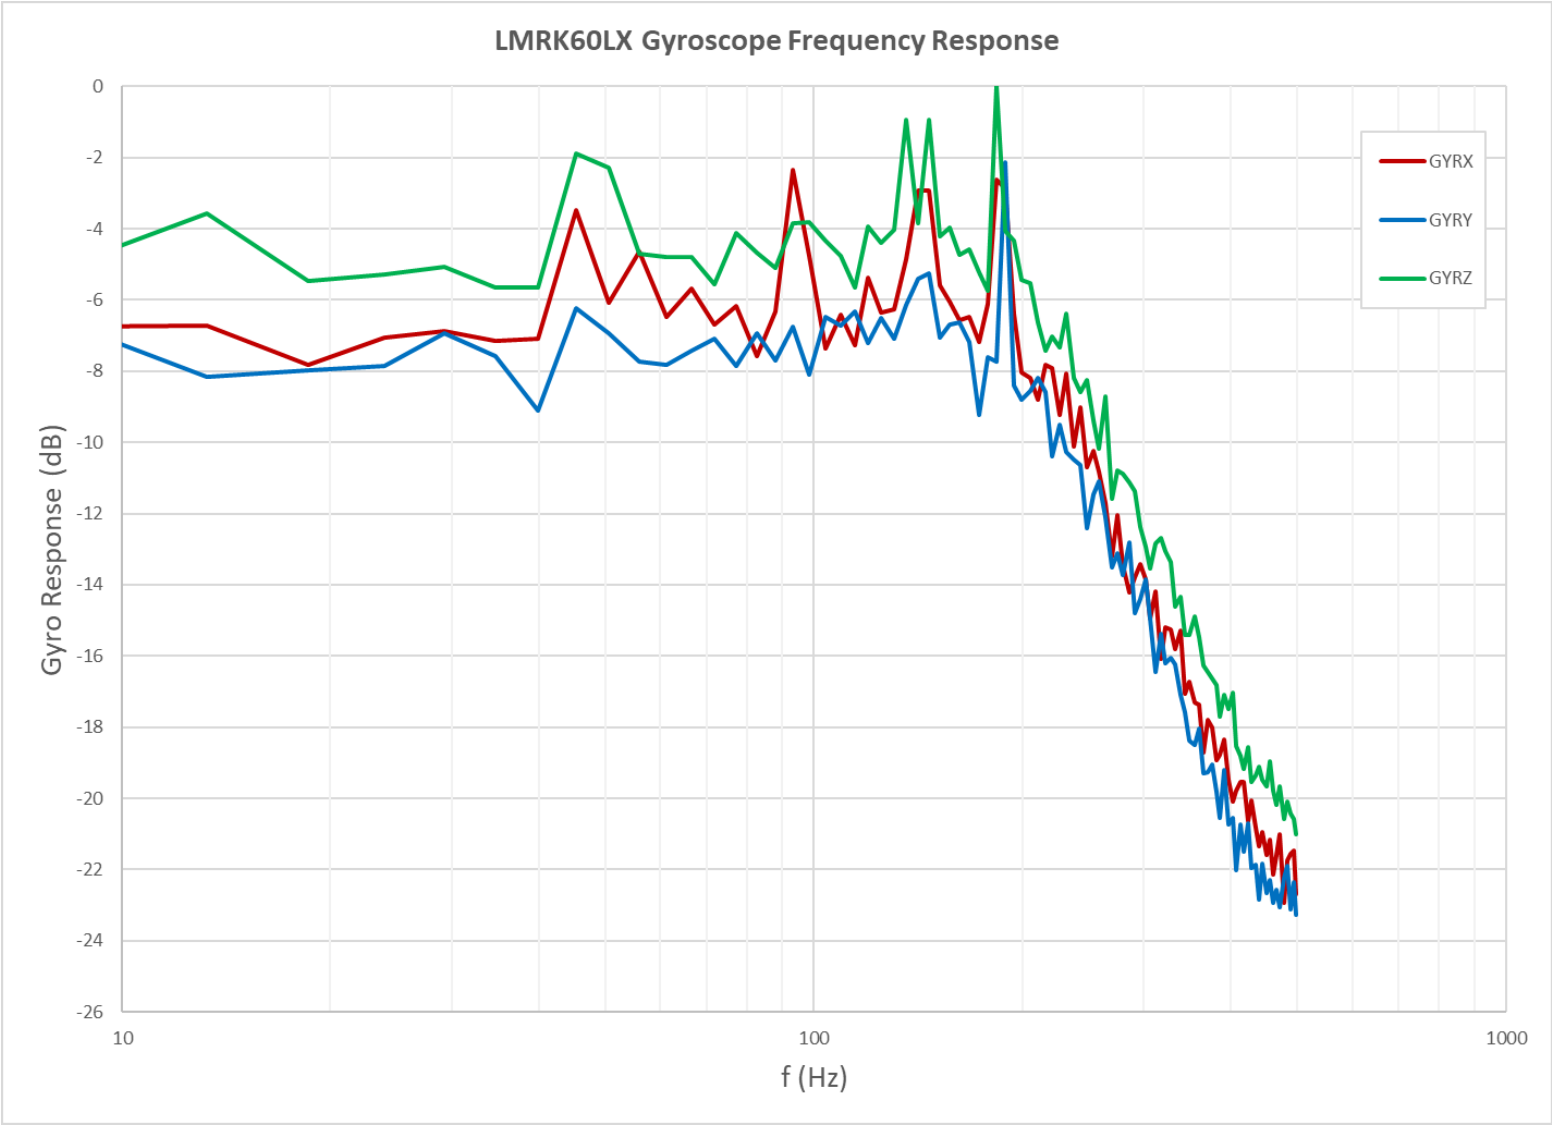

Gyroscope frequency response with LPF set to 250 Hz

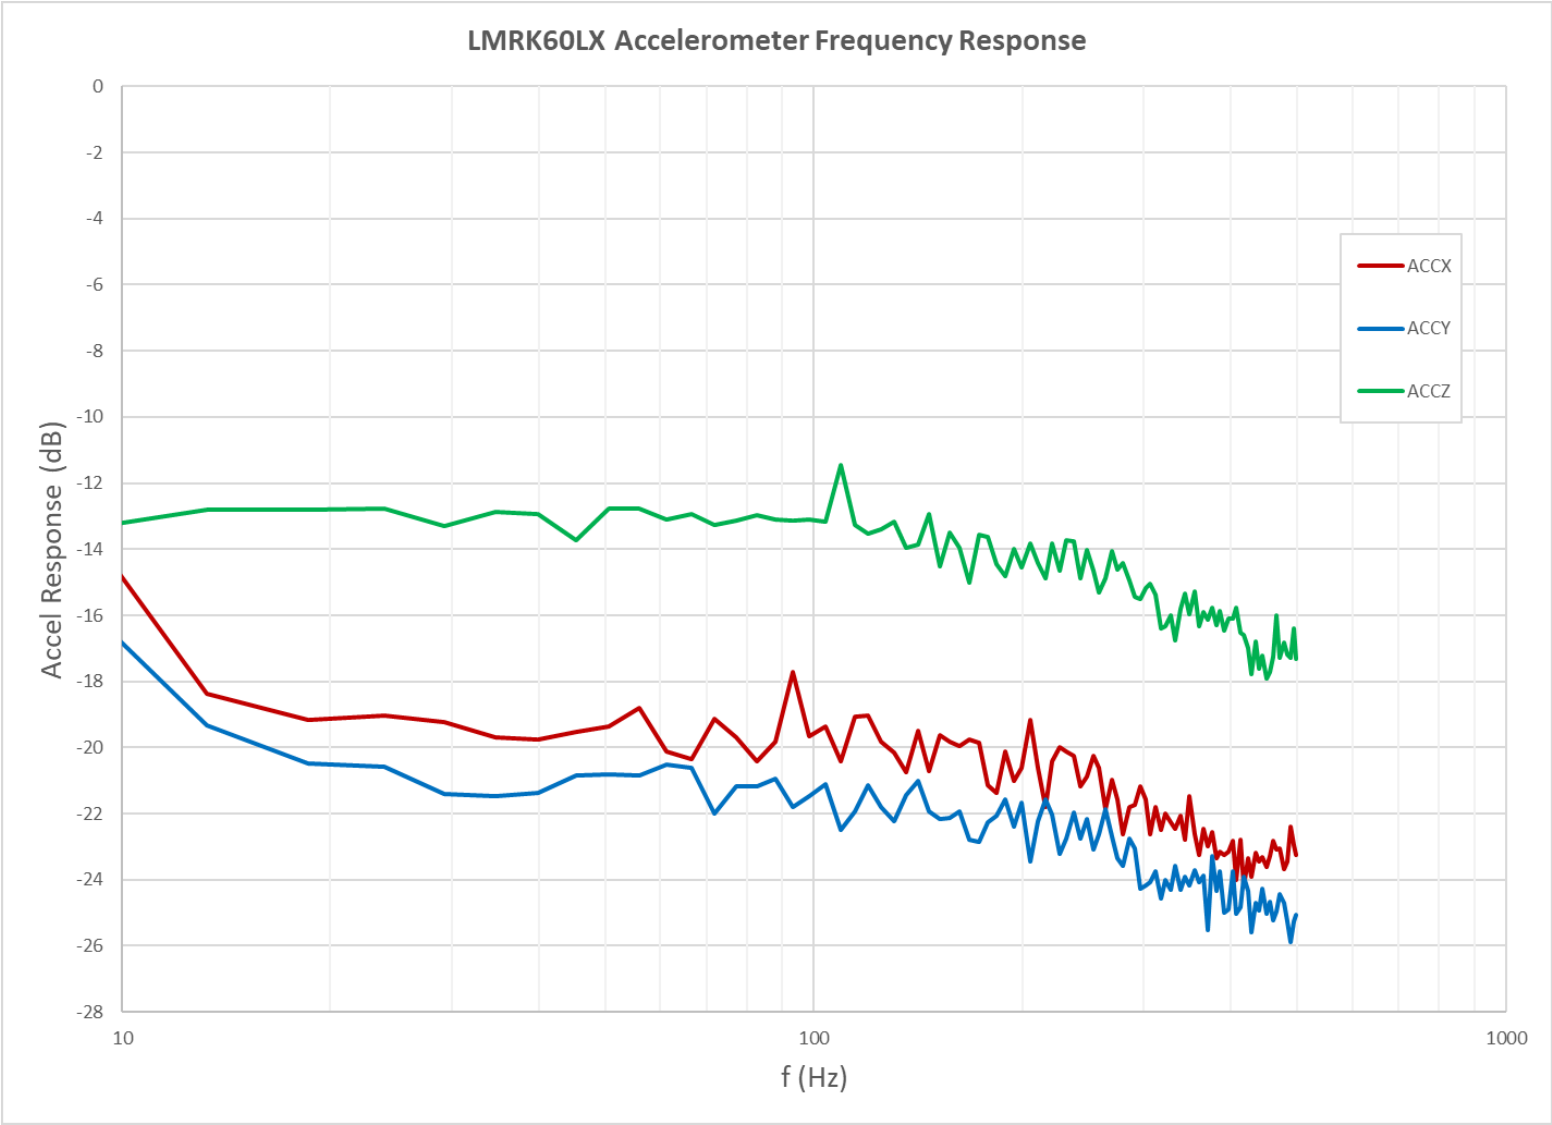

Accelerometer frequency response with LPF set to 250 Hz

