

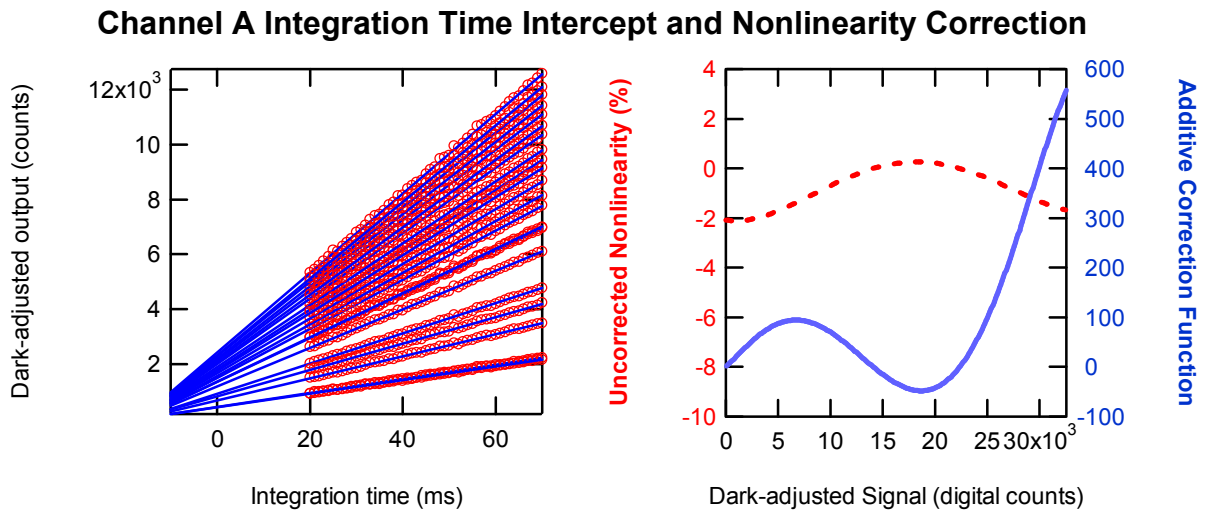



Instrument: HR010424, HydroRad-2 series 200
Calibration Report 2005-12-22 (before cleaning)
Channel A: "Lu_wet" (Radiance, W/m²/sr/nm)

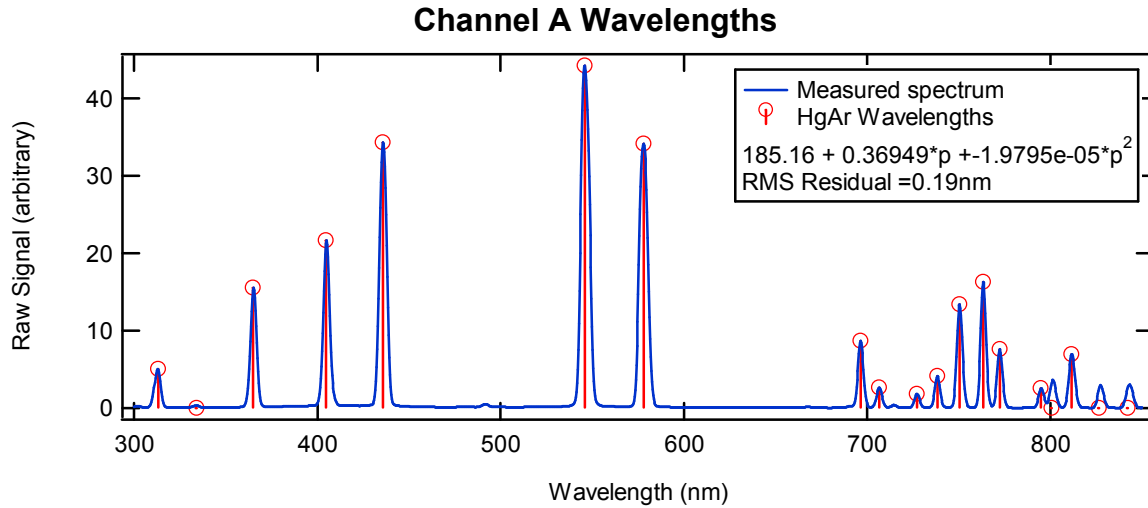


Channel A Radiometric Calibration and Saturation Limit



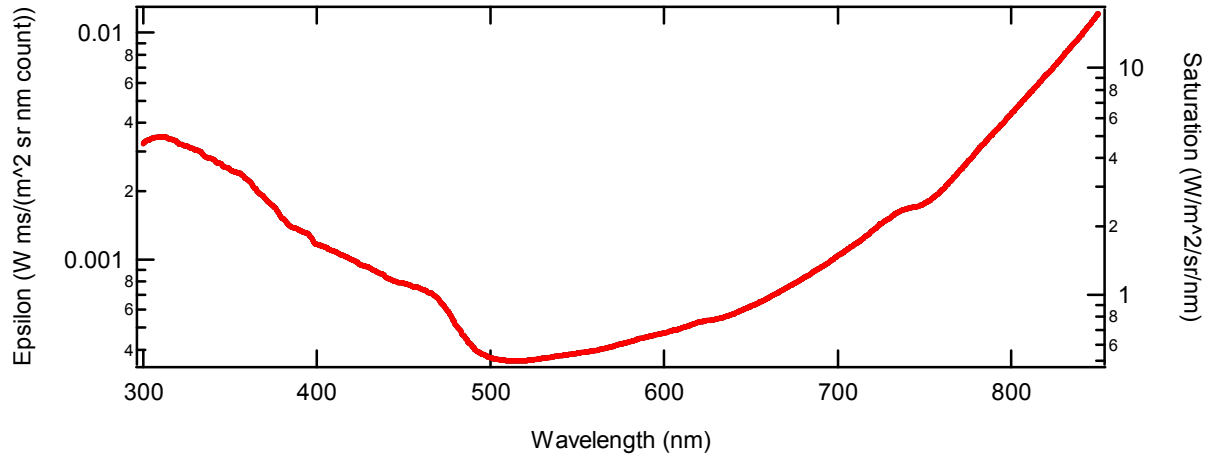


Channel A Comparison to Calibrated Source

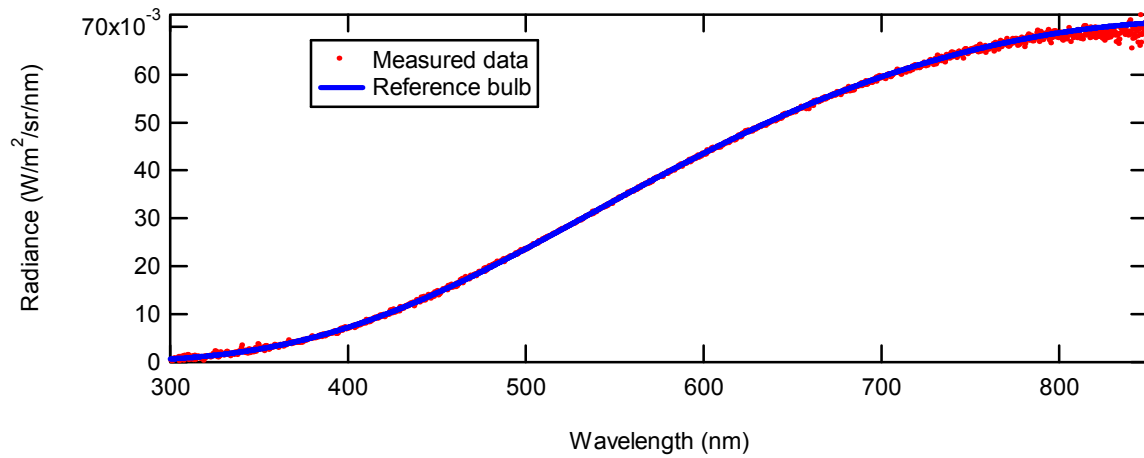


Channel A Immersion Factor

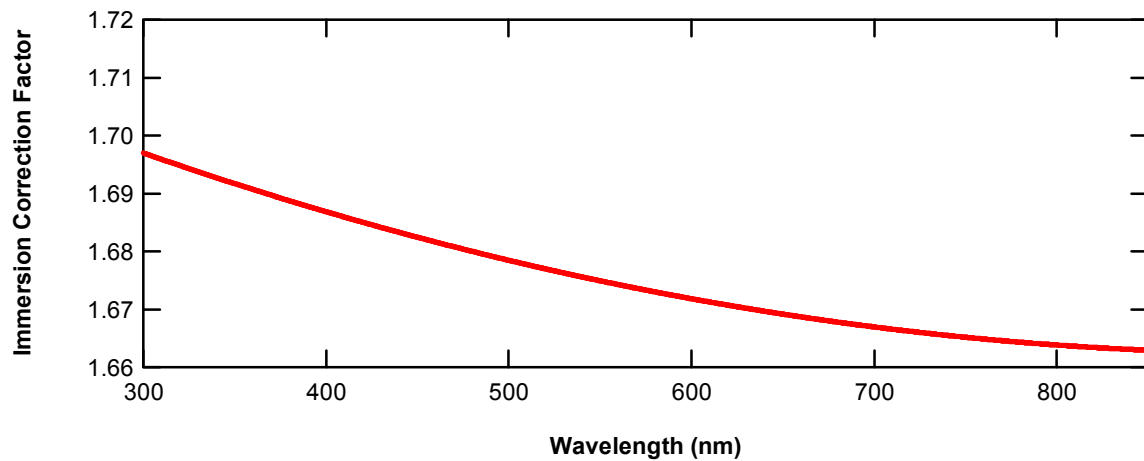

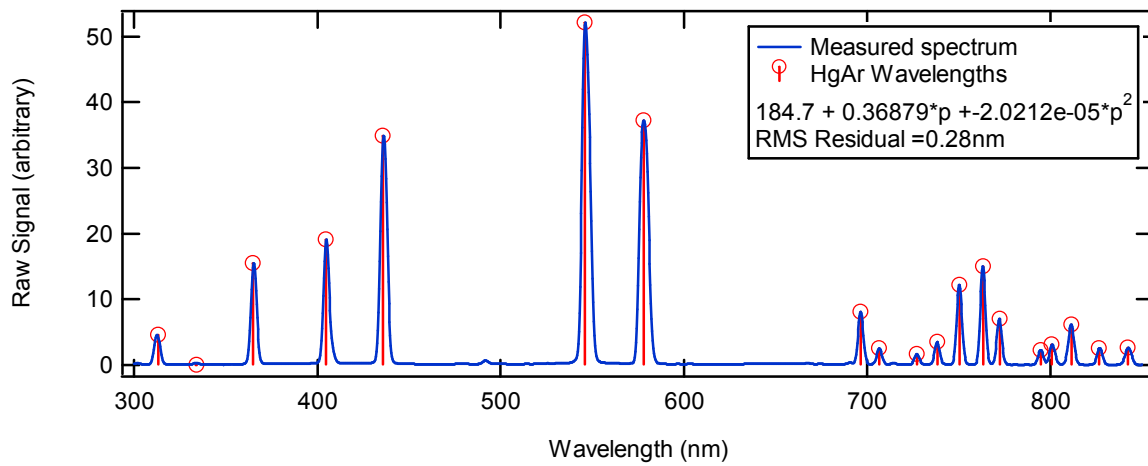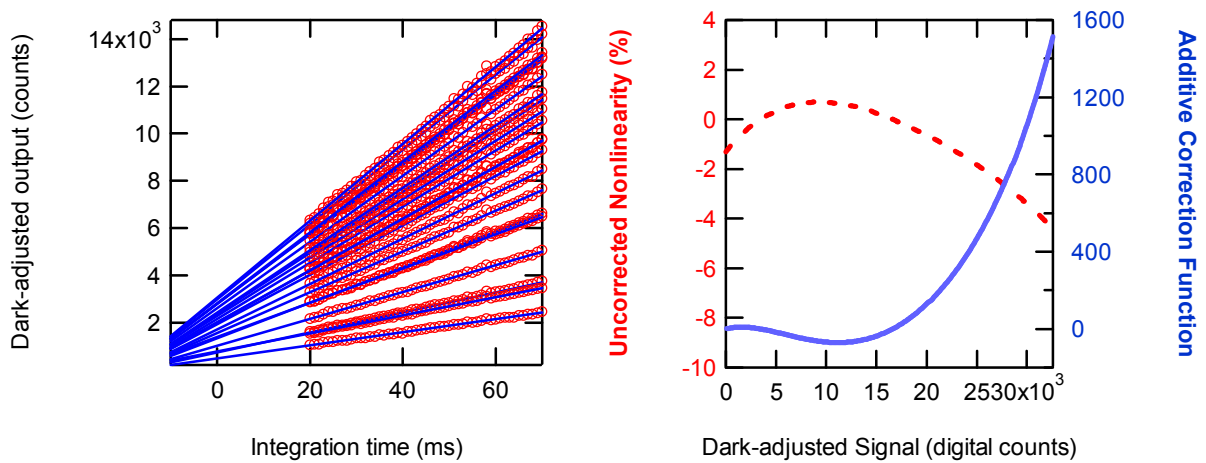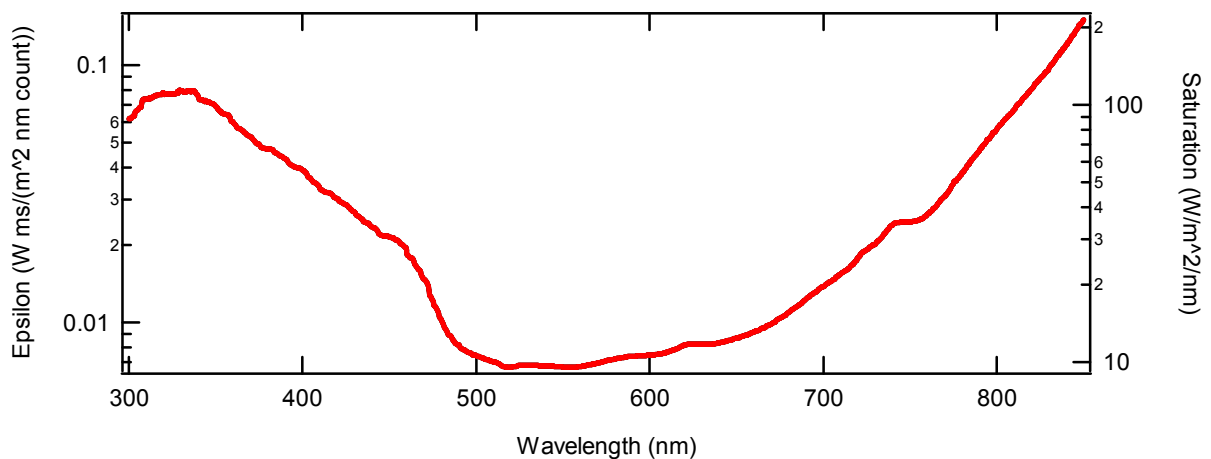Channel B: "Ed_wet" (Irradiance, W/m²/nm)**Channel B Wavelengths****Channel B Integration Time Intercept and Nonlinearity Correction****Channel B Radiometric Calibration and Saturation Limit**

Channel B Comparison to Calibrated Source

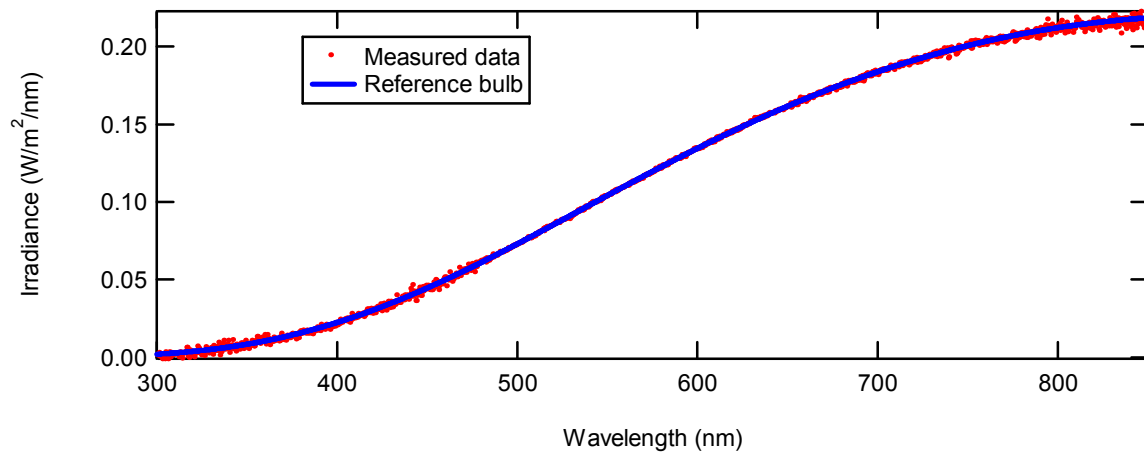

Channel B Immersion Factor

