

HydroScat-2 Calibration Certification

Cert Date: August 5, 2008

Serial Number: H2010334


Configuration: W1B1R0F0S0T1I2

Technician: **SM**

Channel 1: bb420

mu:	17.84
mu Rho:	1.1
SigmaExp:	0.148
TempCoeff:	-0.001778


	Gain Factor	Dark Offset
Gain 1:	1.000	15
Gain 2:	9.462	14
Gain 3:	93.131	16
Gain 4:	942.25	15
Gain 5:	9909.9	5

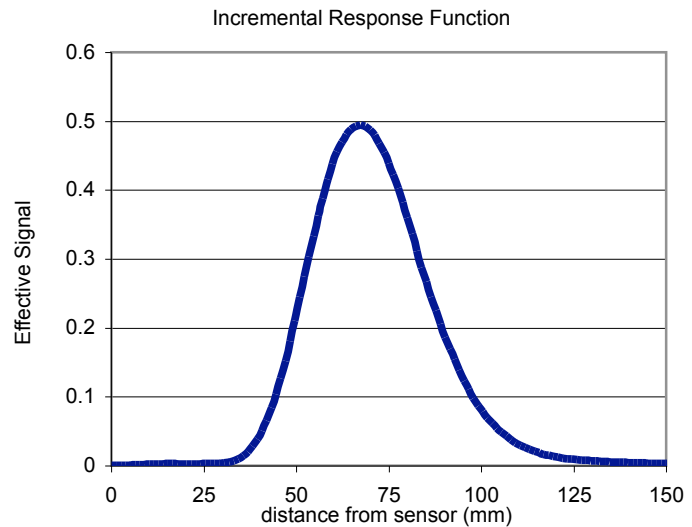


Channel 2: bb700

mu:	11.38
mu Rho:	1.1
SigmaExp:	0.145
TempCoeff:	-0.001625

	Gain Factor	Dark Offset
Gain 1:	1.000	11
Gain 2:	9.542	9
Gain 3:	95.264	5
Gain 4:	937.76	-8
Gain 5:	9942.7	-154

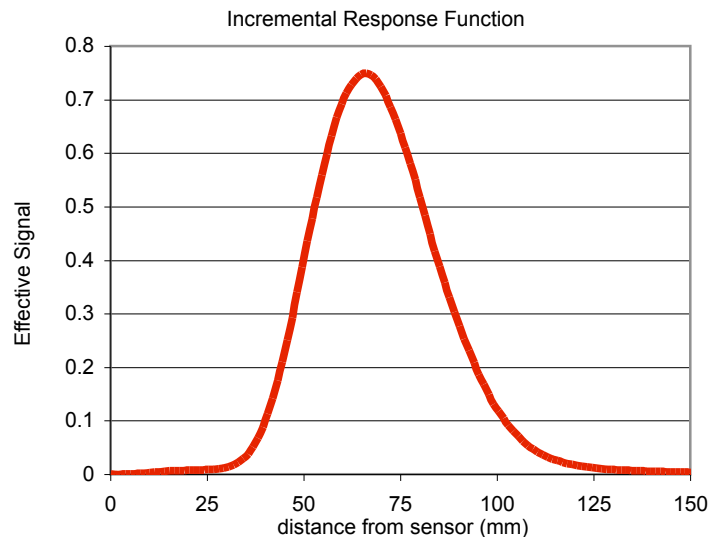



HydroScat-2 Calibration Certification

Cert Date: August 5, 2008

Serial Number: H2010334

Configuration: W1B1R0F0S0T1I2

Depth Calibration

Technician:

SM

Date:

8/5/08

Coefficient:

0.0108

meter / count

Offset:

27.4

meters

