

HydroScat-2 Calibration Certification

Cert Date: **February 6, 2010**

Serial Number: **H2010334**


Configuration: **W1B1R0F0S0T1I2**

Technician: **SM**

Channel 1: bb420

mu:	18.52
mu Rho:	1.1
SigmaExp:	0.147
TempCoeff:	-0.001778


	Gain Factor	Dark Offset
Gain 1:	1.000	12
Gain 2:	9.478	12
Gain 3:	92.857	15
Gain 4:	932.51	14
Gain 5:	9639.9	4

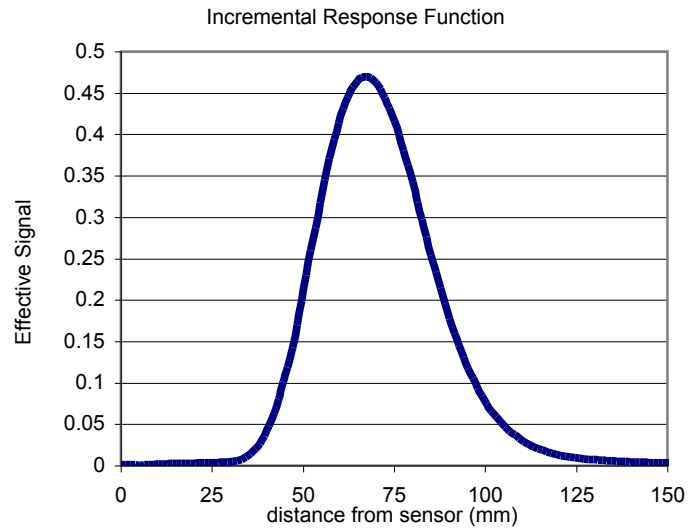


Channel 2: bb700

mu:	11.81
mu Rho:	1.1
SigmaExp:	0.145
TempCoeff:	-0.001625

	Gain Factor	Dark Offset
Gain 1:	1.000	6
Gain 2:	9.505	12
Gain 3:	94.944	8
Gain 4:	936.22	-11
Gain 5:	9842.6	-161

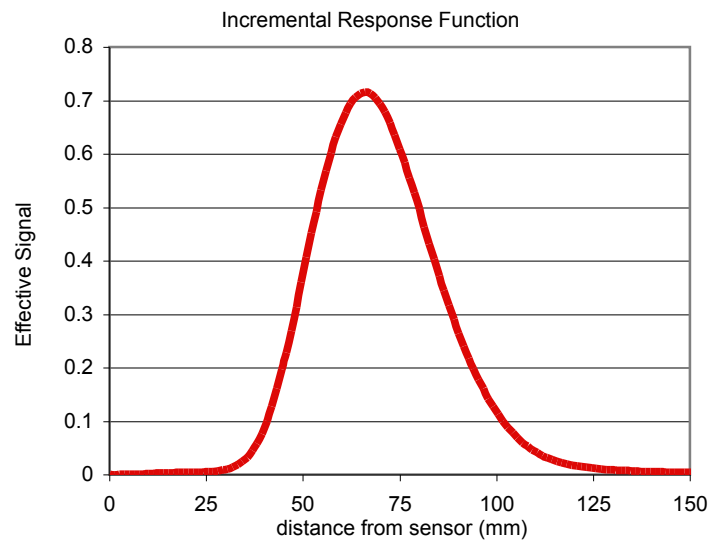



HydroScat-2 Calibration Certification

Cert Date: **February 6, 2010**

Serial Number: **H2010334**

Configuration: **W1B1R0F0S0T112**

Depth Calibration

Technician:

SM

Date:

2/6/10

Coefficient:

0.0108

meter / count

Offset:

27.1

meters

