



Hobi Instrument Services

HydroScat-2 Calibration Certificate

Cert Date: March 29, 2024


Serial Number H2010334

Configuration: W1B1R0F0S0T1I2

Channel 1: bb420

mu:	4.027
mu Rho:	1.1
SigmaExp:	0.142
TempCoeff:	-0.0018


Gain Factor Dark Offset		
Gain 1:	0.106	29
Gain 2:	1.000	27
Gain 3:	9.798	25
Gain 4:	98.02	24
Gain 5:	1009.9	-7

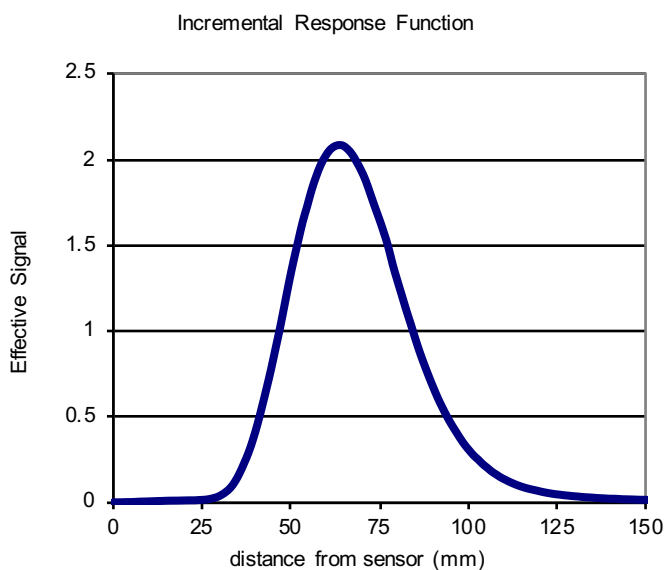

Channel 2: bb700

mu:	14.76
mu Rho:	1.1
SigmaExp:	0.143
TempCoeff:	-0.0016

Gain Factor Dark Offset		
Gain 1:	1.000	24
Gain 2:	9.514	19
Gain 3:	95.333	22
Gain 4:	930.13	0
Gain 5:	9734.1	-141

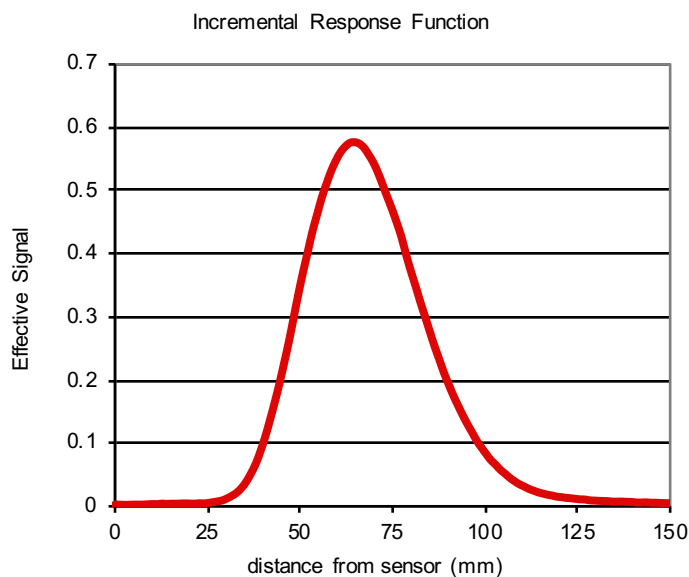



Hobi Instrument Services

Cert Date: **March 29, 2024**
Serial Number **H2010334**
Configuration: **W1B1R0F0S0T1I2**
Depth Cal Dat **1/0/00**

Instrument has no pressure sensor