

HydroScat-2 Calibration Certification

Cert Date: **August 8, 2009**

Serial Number: **H2010336**


Configuration: **W1B1R0F0S0T112**

Technician: **SM**

Channel 1: bb420

mu:	40.73
mu Rho:	1.1
SigmaExp:	0.141
TempCoeff:	-0.00183


	Gain Factor	Dark Offset
Gain 1:	1.000	22
Gain 2:	9.570	27
Gain 3:	95.488	16
Gain 4:	833.42	28
Gain 5:	9469.9	5

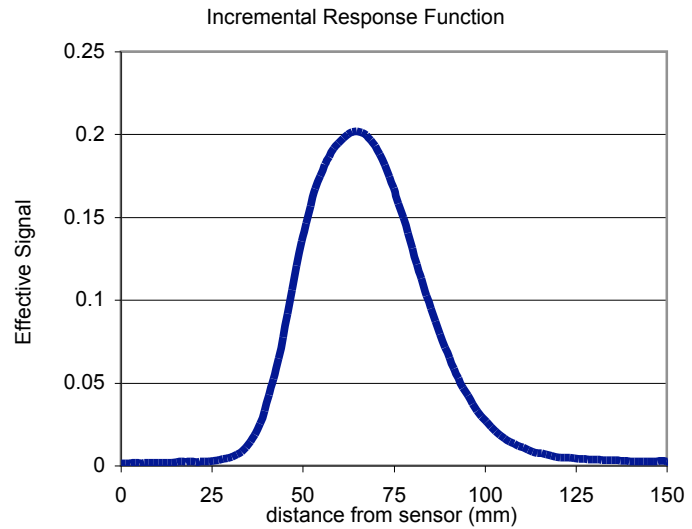


Channel 2: bb700

mu:	9.368
mu Rho:	1.1
SigmaExp:	0.15
TempCoeff:	-0.00183

	Gain Factor	Dark Offset
Gain 1:	1.000	16
Gain 2:	9.515	11
Gain 3:	92.968	13
Gain 4:	921.37	14
Gain 5:	9770.6	-11

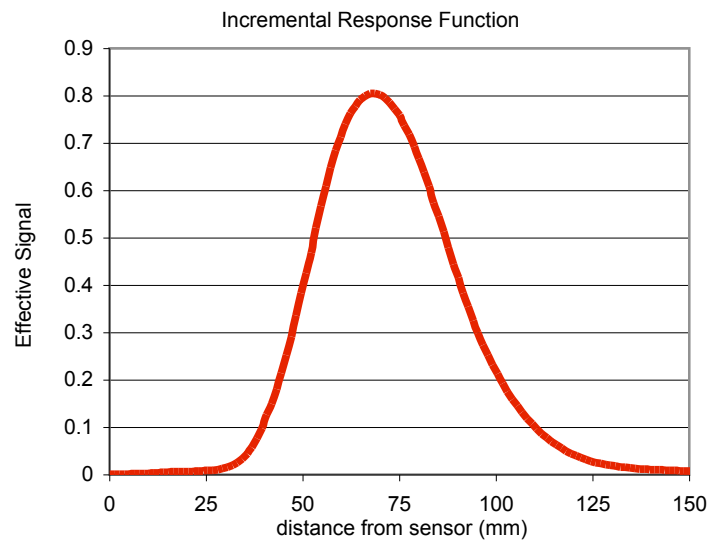



HydroScat-2 Calibration Certification

Cert Date: **August 8, 2009**

Serial Number: **H2010336**

Configuration: **W1B1R0F0S0T1I2**

Depth Calibration

Technician:

0

Date:

1/0/00

Coefficient:

#DIV/0!

meter / count

Offset:

#DIV/0!

meters

