



HydroScat-2 Calibration Certification

Cert Date: August 24, 2008

Serial Number: H2061250


Configuration: B0S0F1T1

Technician: SM

Channel 1: bb420

mu:	43.46
mu Rho:	1.1
SigmaExp:	0.146
TempCoeff:	0


	Gain Factor	Dark Offset
Gain 1:	1.000	10
Gain 2:	9.513	15
Gain 3:	93.804	11
Gain 4:	862.59	1
Gain 5:	9807.4	-202

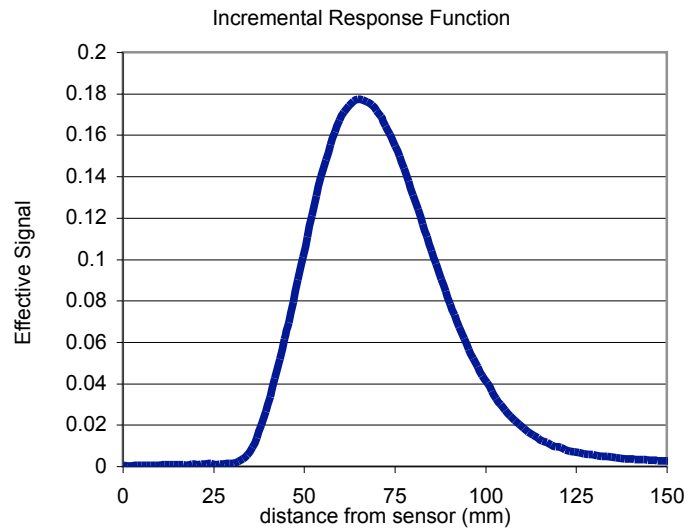


Channel 2: bb700

mu:	9.046
mu Rho:	1.1
SigmaExp:	0.151
TempCoeff:	0

	Gain Factor	Dark Offset
Gain 1:	1.000	10
Gain 2:	9.592	10
Gain 3:	94.309	17
Gain 4:	857.15	8
Gain 5:	8726.9	-998

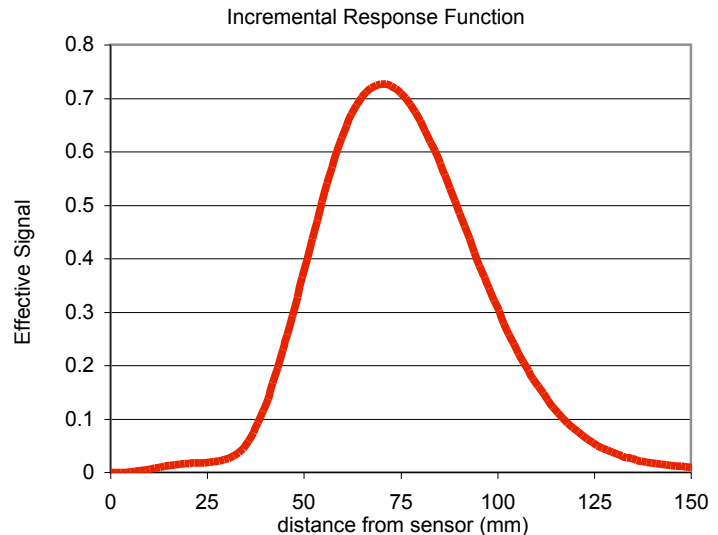



HydroScat-2 Calibration Certification

Cert Date: August 24, 2008

Serial Number: H2061250

Configuration: B0S0F1T1

Depth Calibration

Technician:

SM

Date:

7/24/08

Coefficient:

0.0111

meter / count

Offset:

27.8

meters

