

Sea-Bird Electronics, Inc.

13431 NE 20th Street, Bellevue, WA 98005-2010 USA

Phone: (+1) 425-643-9866 Fax (+1) 425-643-9954 Email: seabird@seabird.com

SENSOR SERIAL NUMBER: 0816
CALIBRATION DATE: 17-Apr-12

SBE 37 RTC CALIBRATION DATA
ITS-90 TEMPERATURE SCALE

COEFFICIENTS:

rtca0 = 9.999797e-001

rtca1 = 1.657233e-006


rtca2 = -2.811963e-008

BATH TEMP (ITS-90)	RTC FREQ (Hz)	COMPUTED FREQ (Hz)	RESIDUAL (PPM)
1.0000	0.9999810	0.9999813	0.3
4.5000	0.9999870	0.9999866	-0.4
15.0000	0.9999980	0.9999982	0.2
18.5000	1.0000010	1.0000007	-0.3
24.0000	1.0000030	1.0000033	0.3
29.0000	1.0000040	1.0000041	0.1
32.5000	1.0000040	1.0000038	-0.2

$$\text{RTC frequency} = \text{rtca0} + \text{rtca1} * t + \text{rtca2} * t^2$$

$$\text{Residual} = (\text{Computed RTC frequency} - \text{Measured RTC frequency}) * 1e6$$

Date, Delta F ppm

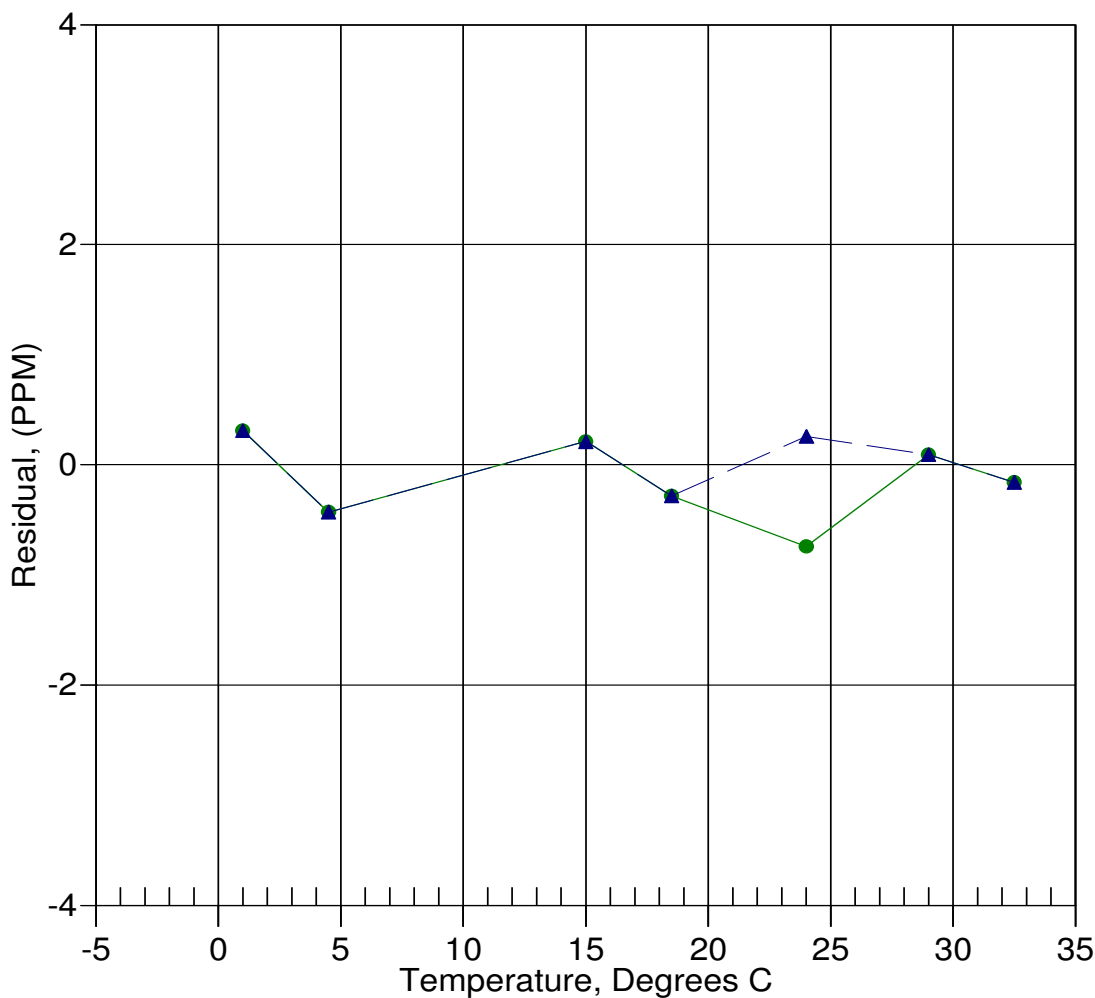

12-Jun-09 -1.00
17-Apr-12 -0.00