


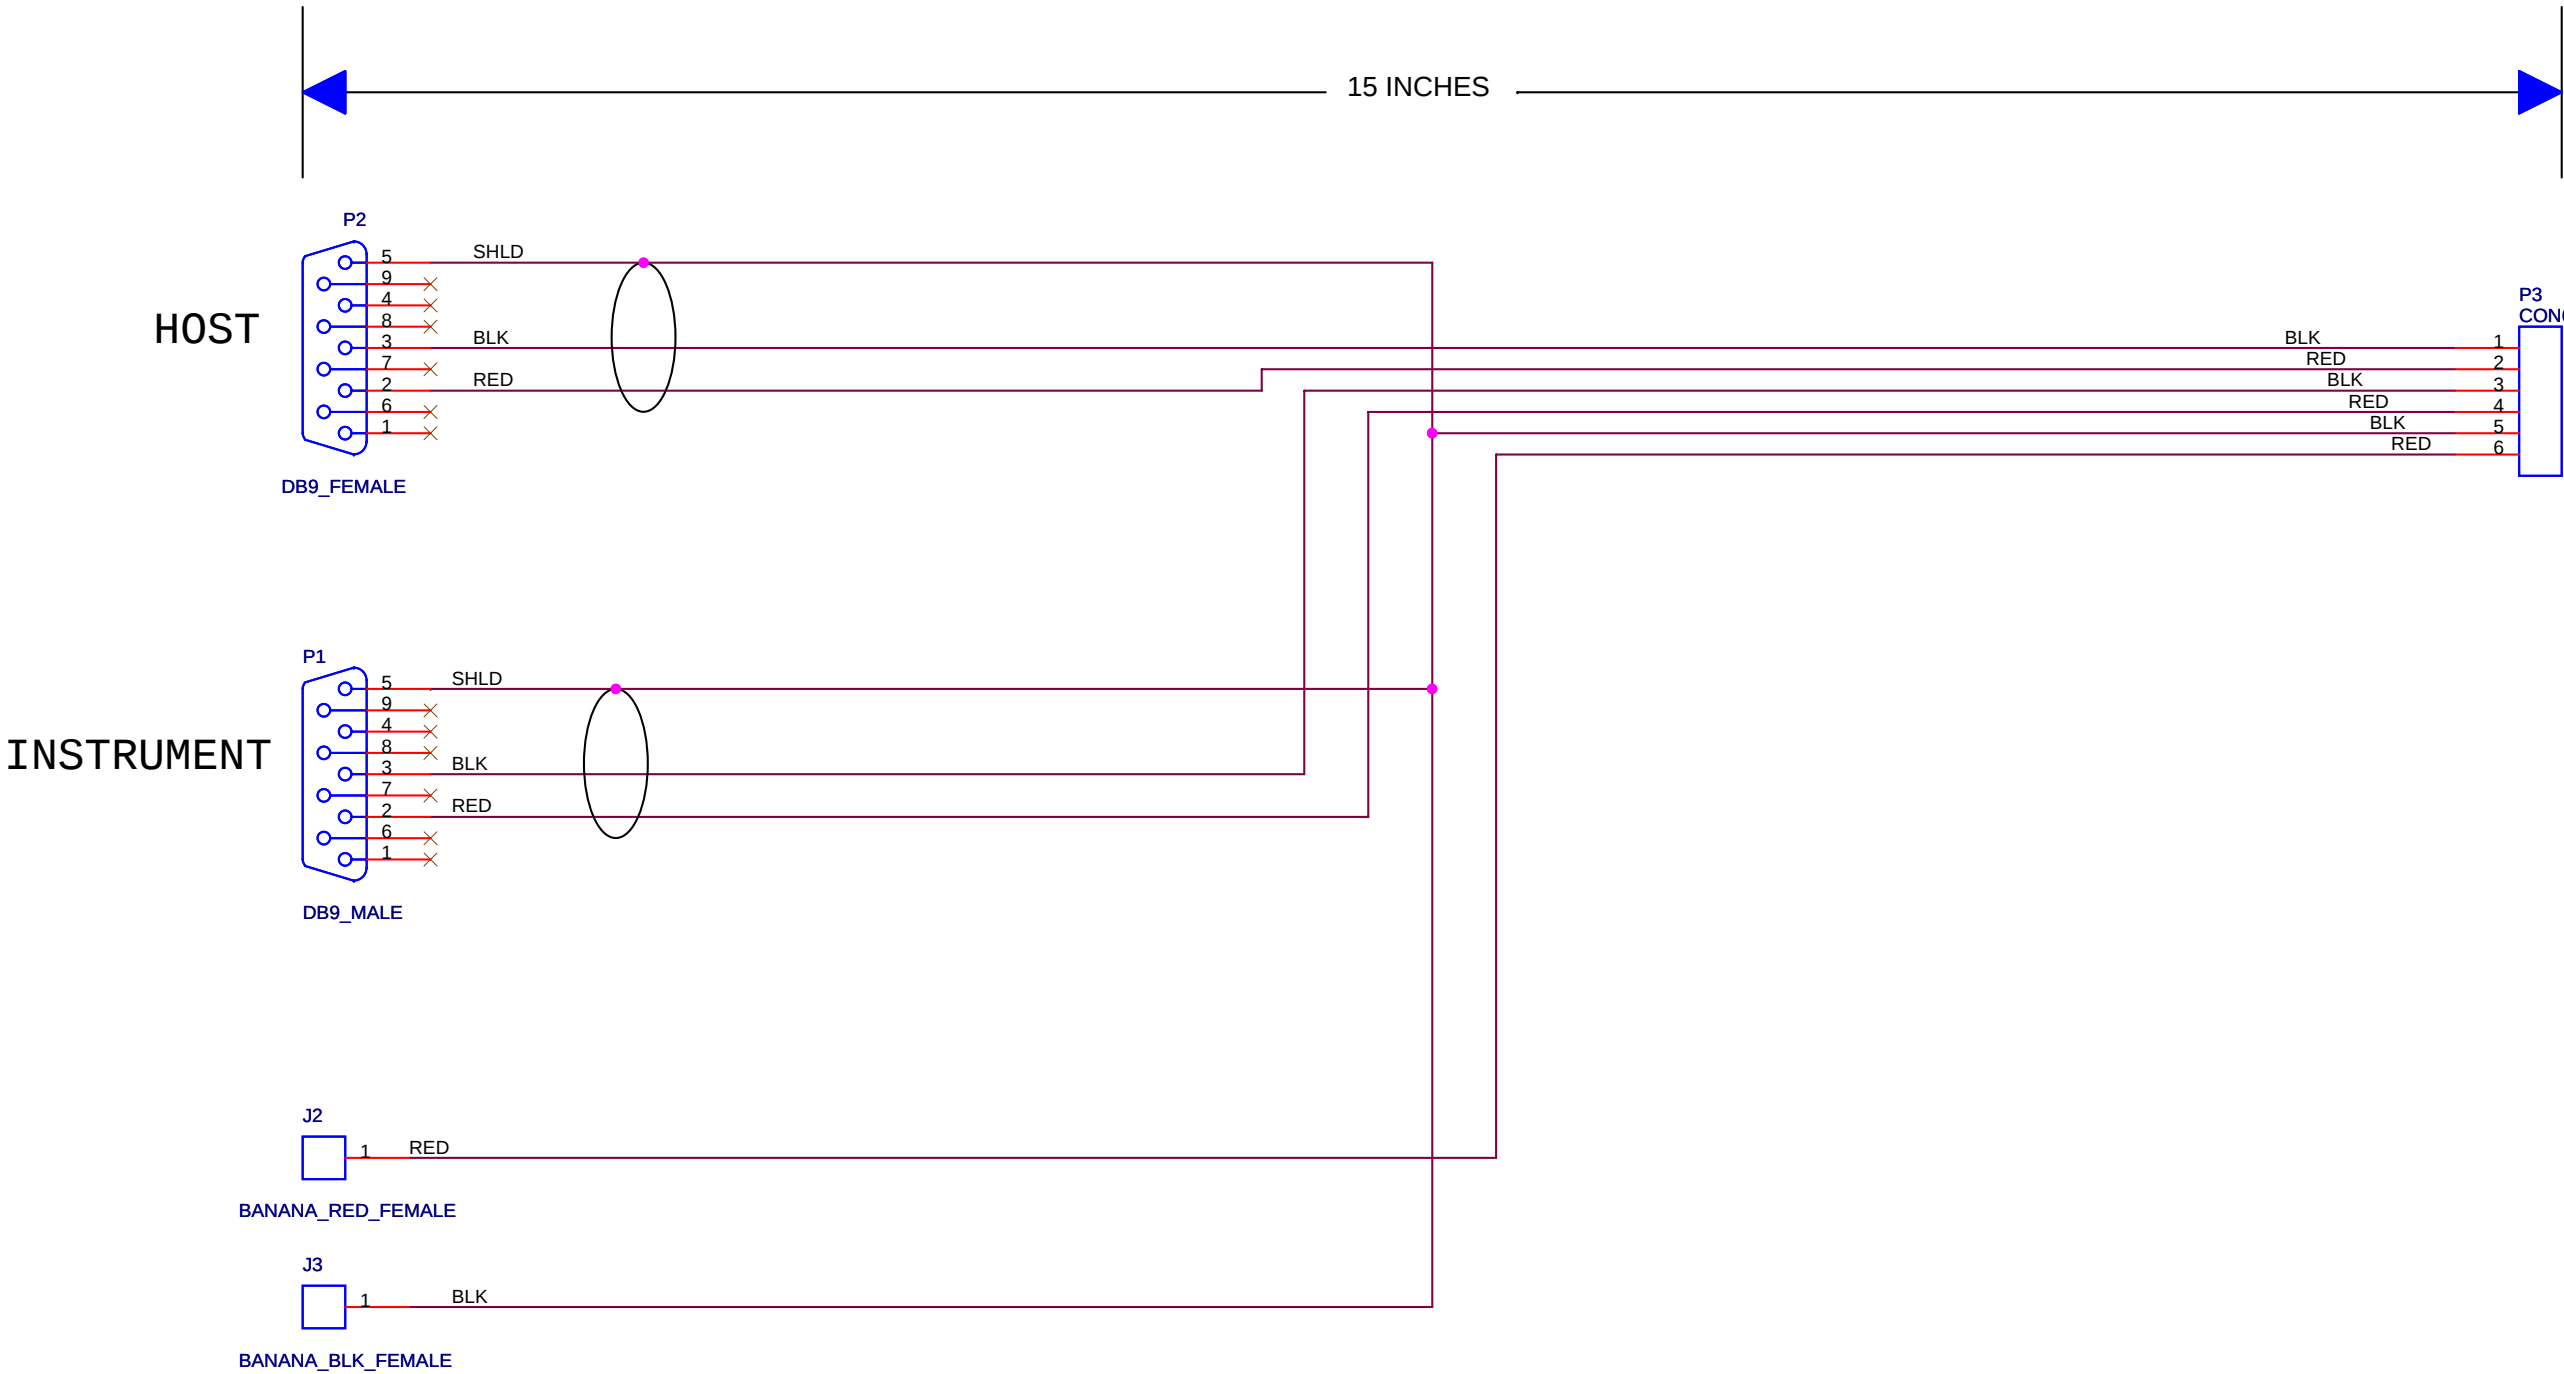

NOTES (Unless otherwise noted):

1. 22 AWG STRANDED WIRE
2. INSTALL HEAT SHRINK TUBING ON ALL SOLDER CONNECTIONS
3. INSTALL PLASTIC SHELLS ON DB9 CONNECTORS
4. ADD LABEL "PUCK LAB TEST CABLE P/N-1002936" TOWARDS P3
5. ADD LABEL "HOST" TOWARDS P2
4. ADD LABEL "INSTRUMENT" TOWARDS P1

		Monterey Bay Aquarium Research Institute 7700 Sandhold Road, Moss Landing, CA 95039	
		Title NON-ISOLATED PUCK TEST CABLE	
Engineer L. MCBRIDE	Size B	Document Number 1002936	Layout File N/A
Layout <Layout>	Date: Friday, January 04, 2008	Sheet 1	of 1
2		1	